

**USER MANUAL**

---

**AUTO REFRACTOMETER  
RM-800**

**AUTO KERATO-REFRACTOMETER  
KR-800**



# INTRODUCTION

Thank you for purchasing the TOPCON Auto Refractometer RM-800, Auto Kerato-Refractometer KR-800.

---

## **INTENDED USE / INDICATIONS FOR USE**

This instrument is used to measure the spherical refractive-power, cylindrical refractive power, the direction of astigmatic axis, the radius of curvature, to compute the corneal refractory power, corneal astigmatic power and the corneal astigmatic axis angle.

(Function to measure the radius of curvature, to compute the corneal refractory power, corneal astigmatic power and the corneal astigmatic axis angle is possible only with KR-800.)

---

## **FEATURES**

**This instrument features the following:**

- The auto shoot function facilitates quick measurements under the optimal condition. (Only in KR-800)
- This instrument is simple to operate and measures the refraction and corneal curvature of the eye. (Function to measure the corneal refraction is possible only with KR-800.)

---

## **PURPOSE OF THIS MANUAL**

This User Manual provides an overview of the basic operation, troubleshooting, checking, maintenance and cleaning of the TOPCON Auto Refractometer RM-800, Auto Kerato-Refractometer KR-800.

To get the best use of the instrument, read Safety Displays and Safety Cautions.

Keep this Manual at hand for future reference.

- 
- Since this product is a precision instrument, always use and keep it in a normally controlled living environment, within a temperature range of 10-40°C, humidity levels between 30-90% and an atmospheric pressure range of 700hPa-1,060hPa.
  - The instrument should also be placed away from direct sunlight.
  - To ensure smooth operation, install the instrument on a level floor free of vibrations. Also, do not place anything on the instrument.
  - Connect all cables properly before using.
  - Use the power at a rated voltage.
  - When not in use, switch off the power source and apply the rubber cap and dust cover.
  - For accurate measurement results, take care to keep the measuring window clean and free of fingerprints, spots and dust.

---

<b>[CAUTION]</b> Federal laws restricts this device to the sale by or on the order of a physician.
--

Since this product partly uses a program derived from IPA Font, using the product is regarded as consent to the IPA Font License Agreement v1.0.  
For the IPA Font License Agreement v1.0, see page 70 or the following URL.  
[http://ipafont.ipa.go.jp/ipa\\_font\\_license\\_v1.html](http://ipafont.ipa.go.jp/ipa_font_license_v1.html)

---

1. No part of this manual may be copied or reprinted, in whole or in part, without prior written permission.
  2. The contents of this manual are subject to change without prior notice and without legal obligation.
  3. The contents of this manual are correct to the best of our knowledge. Please inform us of any ambiguous or erroneous descriptions, missing information, etc.
-

# CONTENTS

INTRODUCTION .....	1
GENERAL SAFETY INFORMATION.....	6
HOW TO READ THIS MANUAL .....	7
GENERAL MAINTENANCE INFORMATION .....	7
USER MAINTENANCE.....	7
CLEANING OF MEASURING WINDOW.....	7
DISCLAIMERS.....	7
DISPLAYS AND SYMBOLS FOR SAFE USE .....	8
DISPLAYS .....	8
SYMBOLS.....	8
POSITIONS OF WARNING AND CAUTION INDICATIONS .....	9
<b>COMPONENTS</b>	
COMPONENT NAMES.....	10
COMPOSITION OF PARTS WHICH CONTACT THE HUMAN BODY .....	10
OPERATION METHOD OF CONTROL PANEL.....	11
CONTROL PANEL COMPONENTS.....	11
FUNCTION BUTTON .....	12
MONITOR SCREEN .....	13
MEASUREMENT SCREEN.....	13
RM-800.....	13
KR-800.....	13
SETTINGS SCREEN.....	14
CORNEA DIAMETER MEASUREMENT SCREEN (ONLY IN KR-800).....	14
PRINTER OUTPUT .....	15
RM-800.....	15
KR-800.....	16
PRINTOUT FORMAT SETTING.....	18
STANDARD ACCESSORIES .....	19
<b>PREPARATIONS</b>	
INSTALLATION .....	20
CONNECTING POWER CABLE .....	20
CONNECTING EXTERNAL I/O TERMINALS .....	21
DATA OUTPUT .....	21
DATA INPUT .....	21
PRINTER PAPER SETTING .....	22
RECOVERY FROM POWER SAVE STATUS.....	23
<b>BASIC OPERATIONS</b>	
PREPARATION BEFORE MEASUREMENT .....	24
TURNING ON THE INSTRUMENT .....	24
SELECTING THE MEASUREMENT MODE (ONLY IN KR-800) .....	24
PATIENT POSITIONING.....	25
AUTO SHOOT MODE MEASUREMENT (ONLY IN KR-800) .....	26
SETTING THE AUTO SHOOT MODE .....	26
ALIGNMENT AND MEASUREMENT .....	27
DISPLAYING MEASUREMENT VALUES.....	30
MANUAL MODE MEASUREMENT .....	31
SETTING THE MANUAL MODE (ONLY IN KR-800) .....	31
ALIGNMENT AND MEASUREMENT .....	31
DISPLAYING MEASUREMENT VALUES.....	33
PRINT-OUT OF MEASUREMENT VALUES .....	33
CLEARING MEASUREMENT VALUES .....	34
DISPLAYING ALL MEASUREMENT DATA .....	35

OPERATION OF AFTER USE.....	36
<b>OPTIONAL OPERATIONS</b>	
DISPLAYING THE PATIENT ID (PATIENT No.) OR OPERATOR ID .....	37
MEASUREMENT OF CORNEA DIAMETER (ONLY IN KR-800) .....	38
MEASUREMENT ON THE ACTUAL IMAGE .....	38
MEASUREMENT ON THE STILL IMAGE .....	40
OUTPUT USING RS-232C .....	41
INPUT USING USB .....	41
OUTPUT USING LAN .....	41
<b>SETTING FUNCTIONS ON SETUP SCREEN</b>	
OPERATING THE SETUP SCREEN.....	42
PREPARATIONS FOR SETTING .....	42
OUTLINE OF SETUP SCREEN OPERATIONS.....	43
RETURNING TO THE MEASUREMENT SCREEN .....	45
LIST OF SETUP ITEMS .....	46
INITIAL (INITIAL SETTING) .....	46
SETTING OF INTERNAL PRINTER (PRINT) .....	48
DATA COMMUNICATION (COMM) .....	50
LAN CONNECTION (LAN) .....	51
OPERATOR ID.....	51
SPECIAL.....	51
<b>MAINTENANCE</b>	
DAILY CHECKUPS.....	52
CHECKING THE MEASURING ACCURACY.....	52
CLEANING THE INSTRUMENT.....	52
CLEANING THE FOREHEAD REST AND CHIN REST.....	52
DAILY MAINTENANCE .....	53
ORDERING CONSUMABLE ITEMS .....	53
USER MAINTENANCE ITEM.....	53
BRIGHTNESS ADJUSTMENT OF CONTROL PANEL.....	54
PRINTER PAPER JAM.....	54
SUPPLYING THE CHINREST TISSUE.....	55
MAINTENANCE .....	56
CLEANING THE KERATO RING AND THE COVER.....	56
CLEANING THE CONTROL PANEL.....	56
<b>TROUBLESHOOTING</b>	
TROUBLE-SHOOTING OPERATIONS .....	57
MESSAGE LIST .....	57
TROUBLE-SHOOTING OPERATIONS.....	58
<b>SPECIFICATIONS AND PERFORMANCE</b>	
SPECIFICATIONS AND PERFORMANCE .....	59
RM-800.....	59
KR-800.....	60
<b>GENERAL INFORMATION ON USAGE AND MAINTENANCE</b>	
INTENDED PATIENT POPULATION .....	61
INTENDED USER PROFILE .....	61
ENVIRONMENTAL CONDITIONS OF USE .....	61
STORAGE, USAGE PERIOD .....	61
ENVIRONMENTAL CONDITIONS FOR PACKAGING IN STORAGE .....	61
ENVIRONMENTAL CONDITIONS FOR PACKAGING IN TRANSPORTATION.....	62
ELECTRIC RATING.....	62
SAFETY DESIGNATIONS PER IEC 60601-1 STANDARD .....	62
DIMENSIONS AND WEIGHT .....	62
OPERATION PRINCIPLE.....	63

DISPOSAL .....	63
ELECTROMAGNETIC COMPATIBILITY .....	64
REQUIREMENTS FOR THE EXTERNAL DEVICE .....	67
PATIENT'S ENVIRONMENT .....	68
<b>REFERENCE</b>	
OPTIONAL ACCESSORIES .....	69
SHAPE OF PLUG .....	69
<b>IPA FONT LICENSE AGREEMENT v1.0</b> .....	70

# GENERAL SAFETY INFORMATION



## WARNINGS

### Ensuring the Safety of Patients and Operators

When operating the instrument, do not touch the patient's eye or nose.

Handling the cord on this product or cords associated with accessories sold with this product, will expose you to lead, a chemical known to the State of California to cause birth defects or other reproductive harm. Wash hands after handling.

### Preventing Electric Shocks and Fires

To avoid fire and electric shock, install the instrument in a dry place free of water and other liquids.

To avoid fire and electric shock, do not put cups or other containers with liquids near the instrument.

To avoid electric shocks, do not insert metal objects into the instrument body through the vent holes or gaps.

To avoid fire in the event of an instrument malfunction, immediately turn OFF the power switch "○" and disconnect the power plug from the outlet if you see smoke coming from the instrument, etc. Don't install the instrument where it is difficult to disconnect the power plug from the outlet. Ask your dealer for service.



## CAUTIONS

### Ensuring the Safety of Patients and Operators

To avoid injury when operating the instrument, do not touch the main body to the patient's eye or nose.

### Preventing Electric Shocks and Fires

To avoid injury by electric shock, do not open the cover. For repair, call your service engineer.

### Electromagnetic Compatibility (EMC)

This instrument has been tested (with 100/120/230V) and found to comply with IEC60601-1-2:Ed.3.0:2007. This instrument radiates radio frequency energy within standard and may affect other devices in the vicinity. If you have discovered that turning on/off the instrument affects other devices, we recommend you change its position, keep a proper distance from other devices, or plug it into a different outlet. Please consult your authorized dealer if you have any additional questions.



# HOW TO READ THIS MANUAL

Read the instructions on pages 1 to 8 before using the machine.

Regarding connection to various devices, see "CONNECTING EXTERNAL I/O TERMINALS" on page 21.

If you would like an overview of the system, begin by reading "BASIC OPERATIONS"(page 24).

For setting various functions, see "SETTING FUNCTIONS ON SETUP SCREEN" on page 42.

## GENERAL MAINTENANCE INFORMATION

### USER MAINTENANCE

To maintain the safety and performance of the equipment, never attempt to repair or perform maintenance. These tasks should be performed by an authorized service representative.

Maintenance tasks that can be performed by the user are as follows; for details, follow the manual's instructions.

### **CLEANING OF MEASURING WINDOW**

For details, See "CLEANING THE INSTRUMENT" on page 52.




## DISCLAIMERS

- TOPCON is not responsible for damage due to fire, earthquakes, actions or inactions of third persons or other accidents, or damage due to negligence and misuse by the user and any use under unusual conditions.
- TOPCON is not responsible for damage derived from inability to properly use this equipment, such as loss of business profits and suspension of business.
- TOPCON is not responsible for damage caused by operations other than those described in this User Manual.
- The device does not provide a diagnosis of any condition or lack thereof or any recommendations for appropriate treatment. The relevant healthcare provider is fully responsible for all diagnosis and treatment decisions and recommendations.









# DISPLAYS AND SYMBOLS FOR SAFE USE

In order to encourage the safe use of the instrument and to avoid danger to the operator and others as well as damage to properties, warnings are described in the User Manual and marked on the instrument body. We suggest you thoroughly understand the meaning of the following displays/icons and Safety Cautions, as well as read the Manual, and strictly observe the instructions.

## DISPLAYS

DISPLAY	MEANING
 <b>WARNING</b>	A WARNING is provided to alert the user to potential serious outcomes (death, injury, or serious adverse events) to the patient or the user.
 <b>CAUTION</b>	A CAUTION is provided to alert the user to use special care necessary for the safe and effective use of the device. They may include actions to be taken to avoid effects on patients or users that may not be potentially life threatening or result in serious injury, but about which the user should be aware. Cautions are also provided to alert the user to adverse effects on this device of use or misuse and the care necessary to avoid such effects.
 <b>NOTES</b>	A NOTE is provided when additional general information is applicable.


## SYMBOLS





Symbol	IEC/ISO Publication	Description	Description (French)
	IEC 60417-5032	Alternating Current	Courant alternatif
	IEC 60417-5008	Off (power: disconnection from the main power supply)	Éteint (courant: coupure avec le secteur)
	IEC 60417-5007	On (power: connection to the main power supply)	Allumé (courant: raccordement sur le secteur)
	IEC 60878-02-02	Type B applied part	Partie appliquée du Type B
	ISO 7010-W001	General warning sign	Symbole d'avertissement général
	ISO 7010-M002	Refer to instruction manual/ booklet	Voir le manuel/la brochure
	ISO 7000-2497	Date of manufacture	Date de fabrication
	ISO 7000-2498	Serial number	Numéro de série

# POSITIONS OF WARNING AND CAUTION INDICATIONS

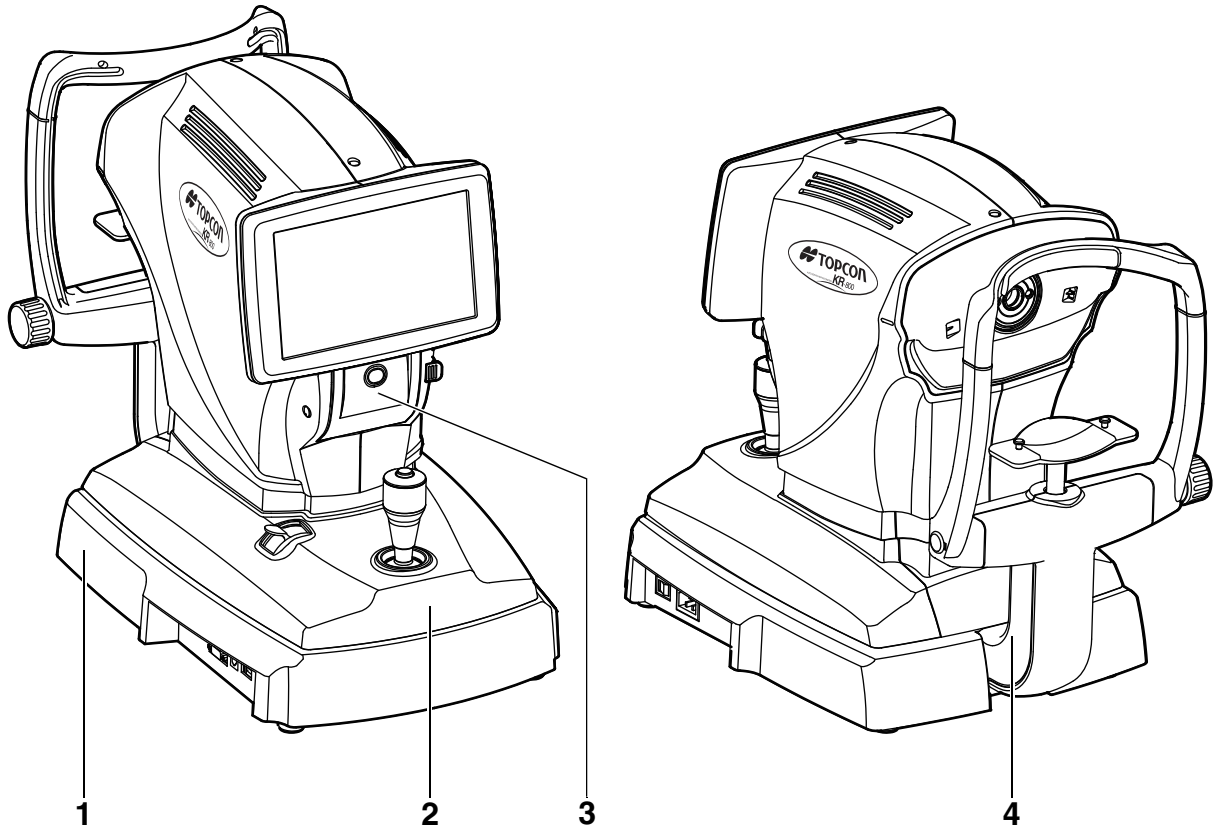To secure safety, this equipment provides warnings.



Correctly use the equipment following these warning instructions. If any of the following marking labels are missing, please contact your dealer or TOPCON at the address stated on the back cover.




No.	Label	Meaning
1		<b>WARNING</b> To avoid injury caused by electric shock, do not open the cover. Ask your dealer for service.
2		<b>CAUTION</b> Be careful not to hit the patient's eyes or nose with the instrument during operation.
3		<b>CAUTION</b> Pay much attention not to touch the internal printer's body when the cover is open. If touched, it may result in trouble due to electrostatic discharge.
4		Degree of protection against electric shock: TYPE B APPLIED PART

# COMPONENTS

## COMPONENT NAMES

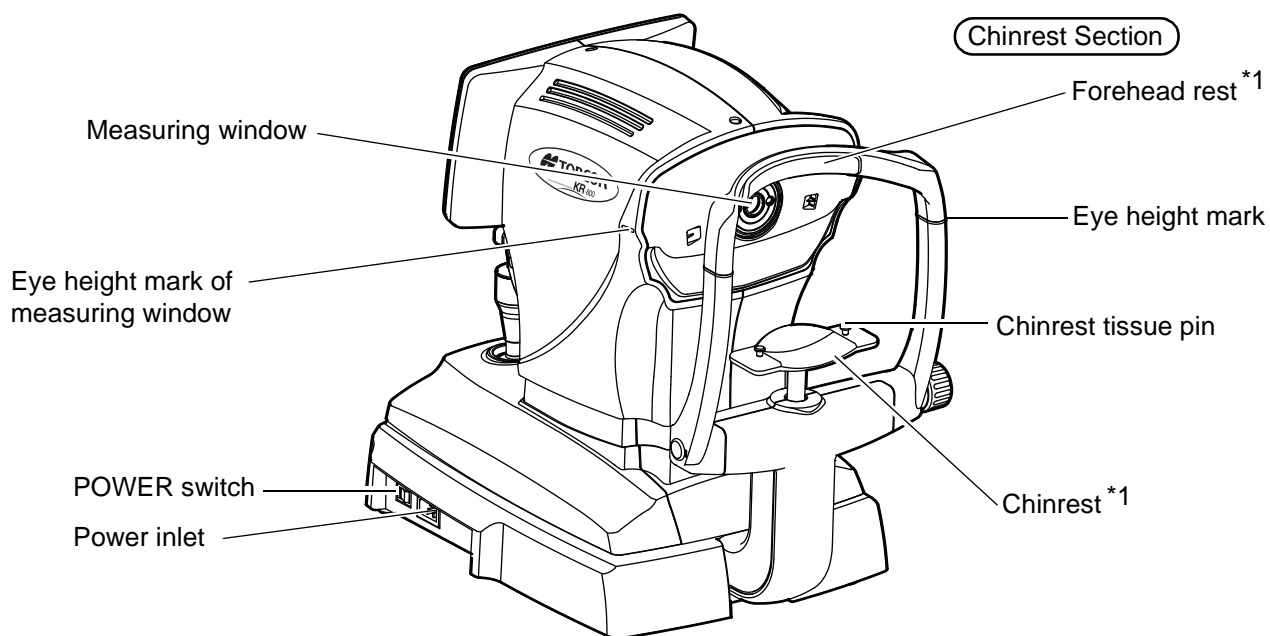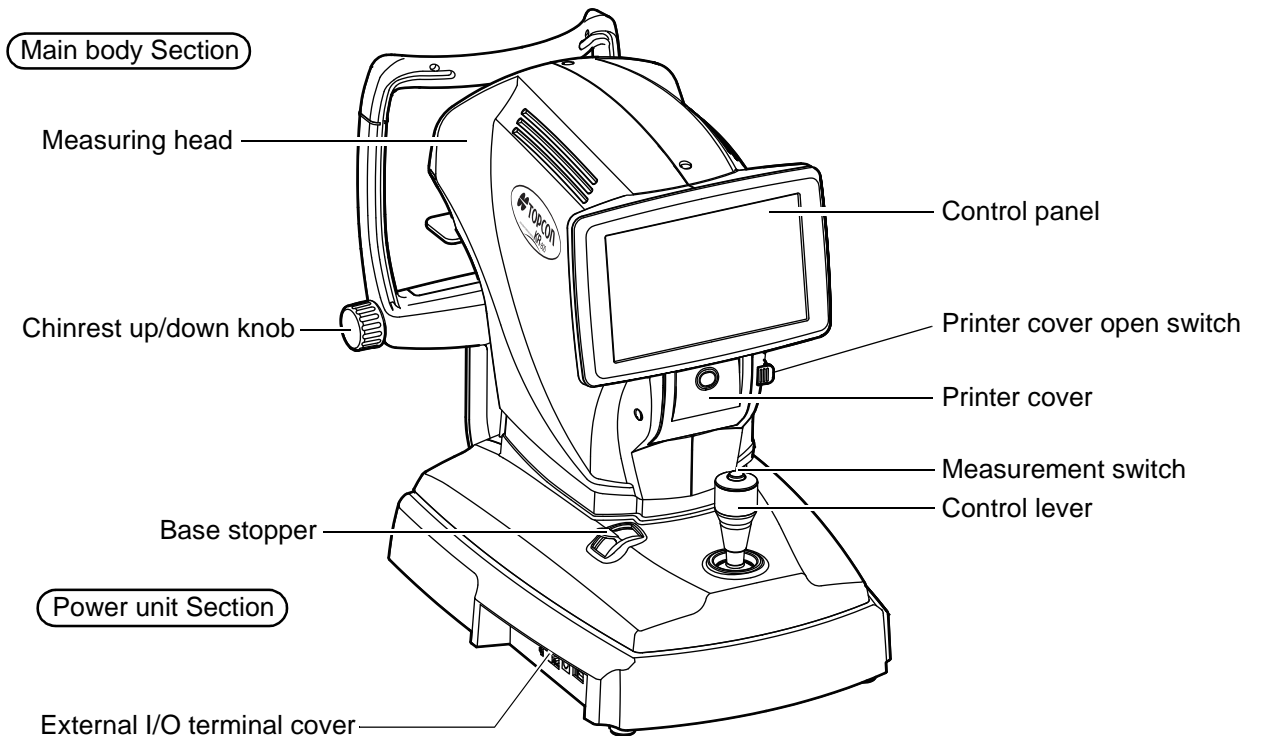


\*1: Contacting part (class B)




## COMPOSITION OF PARTS WHICH CONTACT THE HUMAN BODY

Forehead rest : Silicone rubber  
 Chinrest : Acrylonitrile butadiene styrene resin

# OPERATION METHOD OF CONTROL PANEL

 <b>NOTE</b>	<ul style="list-style-type: none"> <li>• The control panel is a touch panel. Do not use any sharp tools; e.g. ball point pen.</li> <li>• Do not touch two points on a control panel simultaneously.</li> </ul>
---	--


Tap → To select any relevant item.

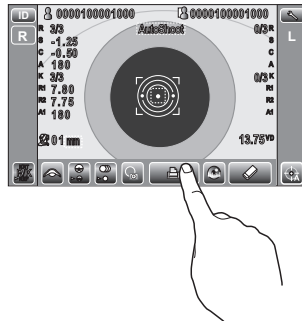




Touch the control panel softly with a finger.

## CONTROL PANEL COMPONENTS

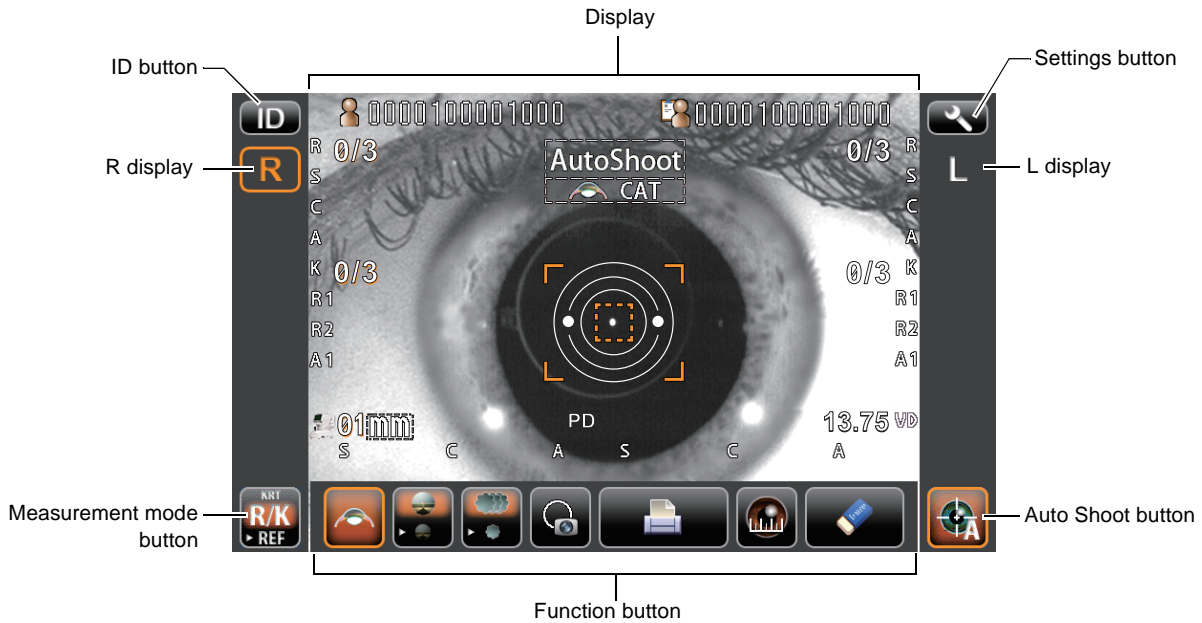The control panel is designed as a touch panel for performing various operations and settings. It displays images and shows information, including set conditions and measurement results.



-  ID button .....Input the patient ID (up to 13 characters) and operator ID (up to 13 characters). However, if no patient ID is input, the patient No. is allocated automatically.
-  Measurement mode button .....Selects a measurement mode from REF, KRT and R/K. (Only in KR-800)
-  R display/L display .....Shows the measured eye is R (Right eye) or L (Left eye). The measured eye is framed in orange.



Auto Shoot button .....Selects Auto Shoot/Manual mode.

When selected, "Auto Shoot" is displayed on the control panel, and this button is framed in orange. (Only in KR-800)



Settings button .....Displays the Settings screen.

## FUNCTION BUTTON



Cataract button

Fixation target button

FOG button

Target image button

Print out button

ALL CLEAR button  
Cornea diameter



Cataract button .....If error messages occur in patient's with cataracts, push the Cataract button may improve measurements. When the button is selected, "CAT" is displayed on the control panel and the selected button is framed in orange.



Fixation target button .....Brightness of the fixation target can be changed.




FOG button .....Changes setting temporarily to perform fogging only in the first measurement or each time in the continuous measurement.



Target image button .....The captured measurement target can be observed on the control panel.



Print out button .....Prints measurement results. Tap the button when no measurement data is present to feed the paper. By setting the printer mode to Graphic Printer on the Settings screen, figures showing refractive conditions can be printed.

In this case, the printer button changes to  .



Cornea diameter button .....Changes to cornea diameter measurement mode. (Only in KR-800)




ALL CLEAR button .....Clears all measurement data.


# MONITOR SCREEN

## MEASUREMENT SCREEN


### RM-800

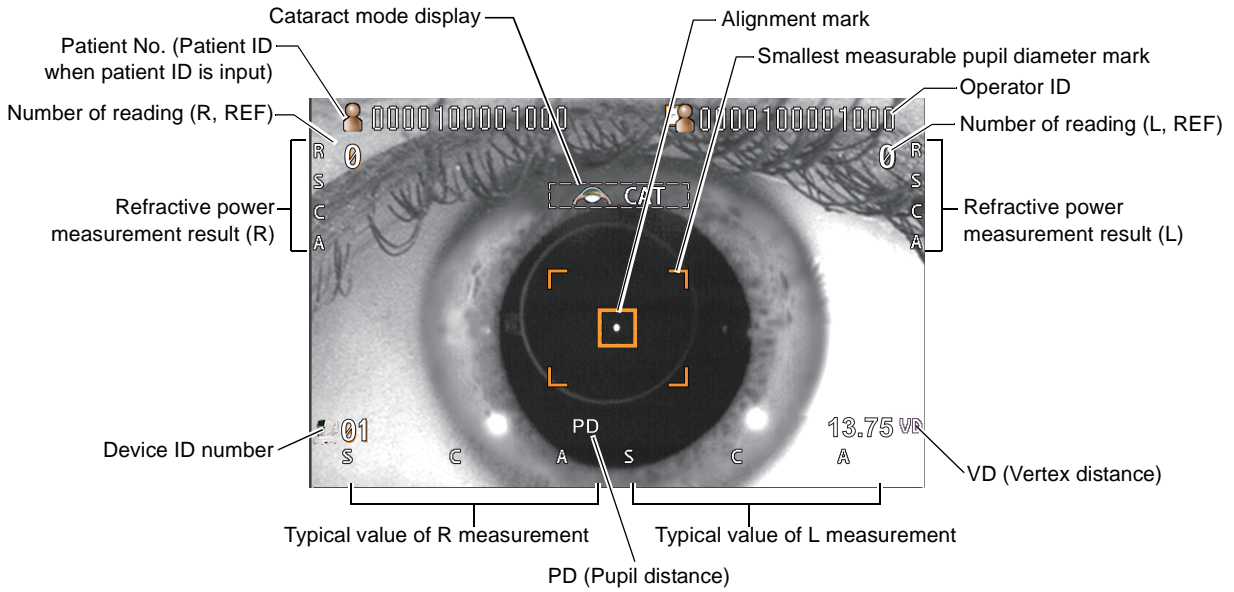


### KR-800

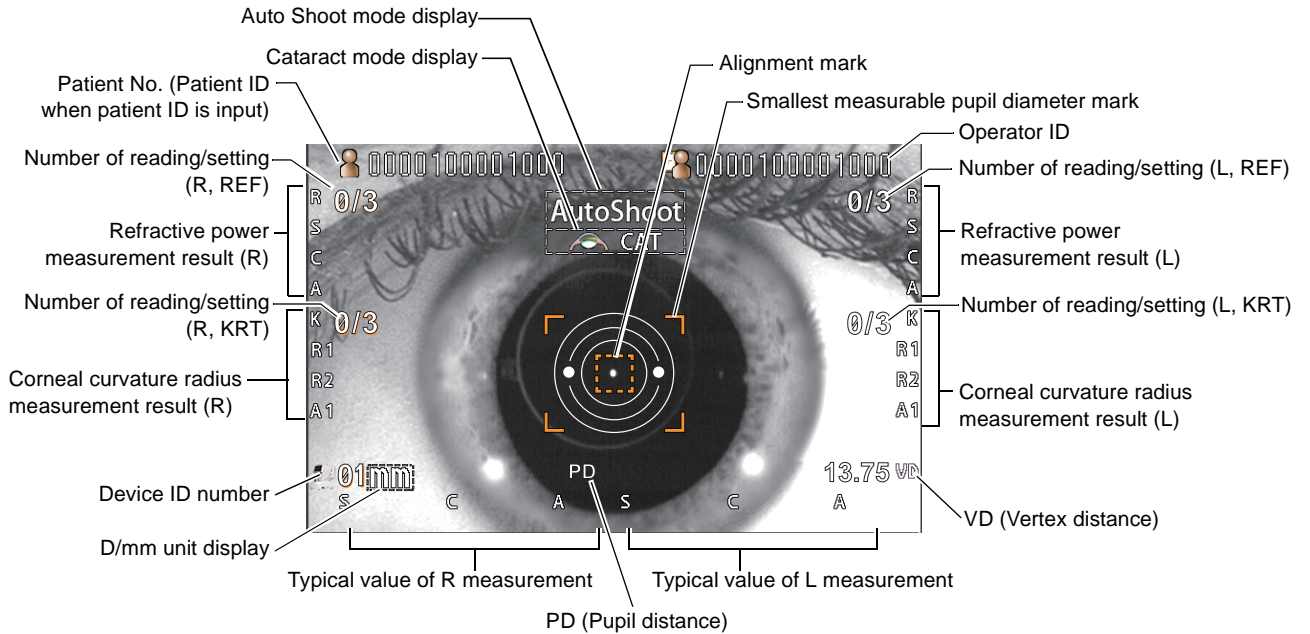

## SETTINGS SCREEN

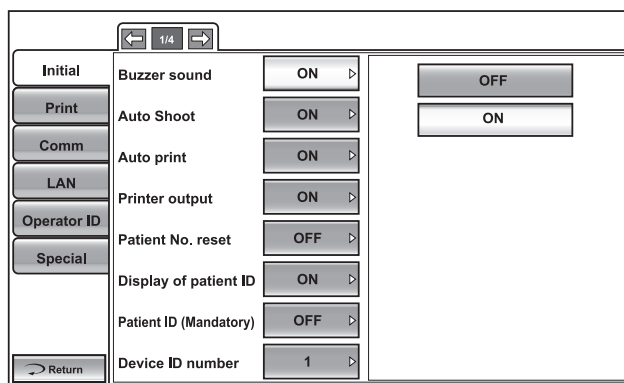


## CORNEA DIAMETER MEASUREMENT SCREEN (ONLY IN KR-800)

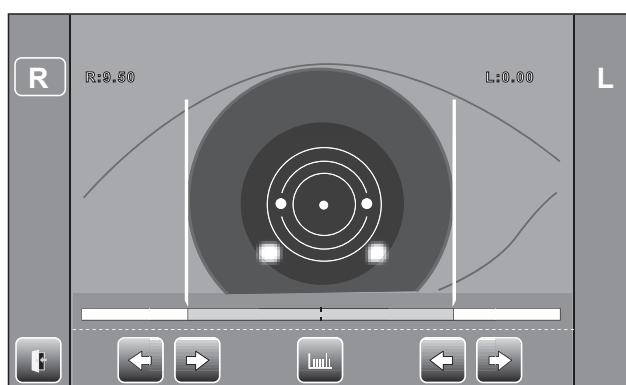




# PRINTER OUTPUT


RM-800

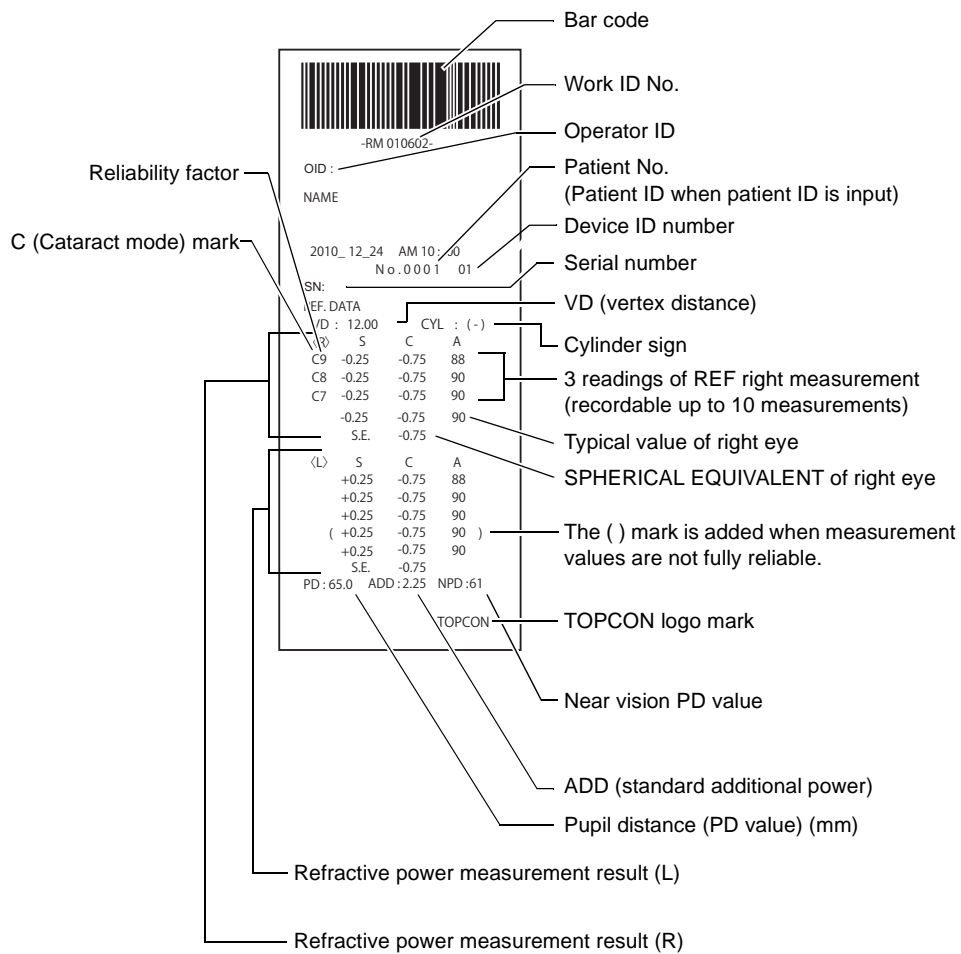


 <b>NOTE</b>	<ul style="list-style-type: none"> <li>The reliability factor is defined with integers 1 to 9 in increasing order of reliability. Additionally, if the reliability is high enough, the reliability factor is not shown on the printout.</li> <li>The Near PD value is calculated based on the ADD.</li> <li>( ) appears when normal measurement is not expected due to eyelid, eyelash, or blinking.</li> </ul>
---	---

**KR-800**

KRT typical value style and KRT print data are HV

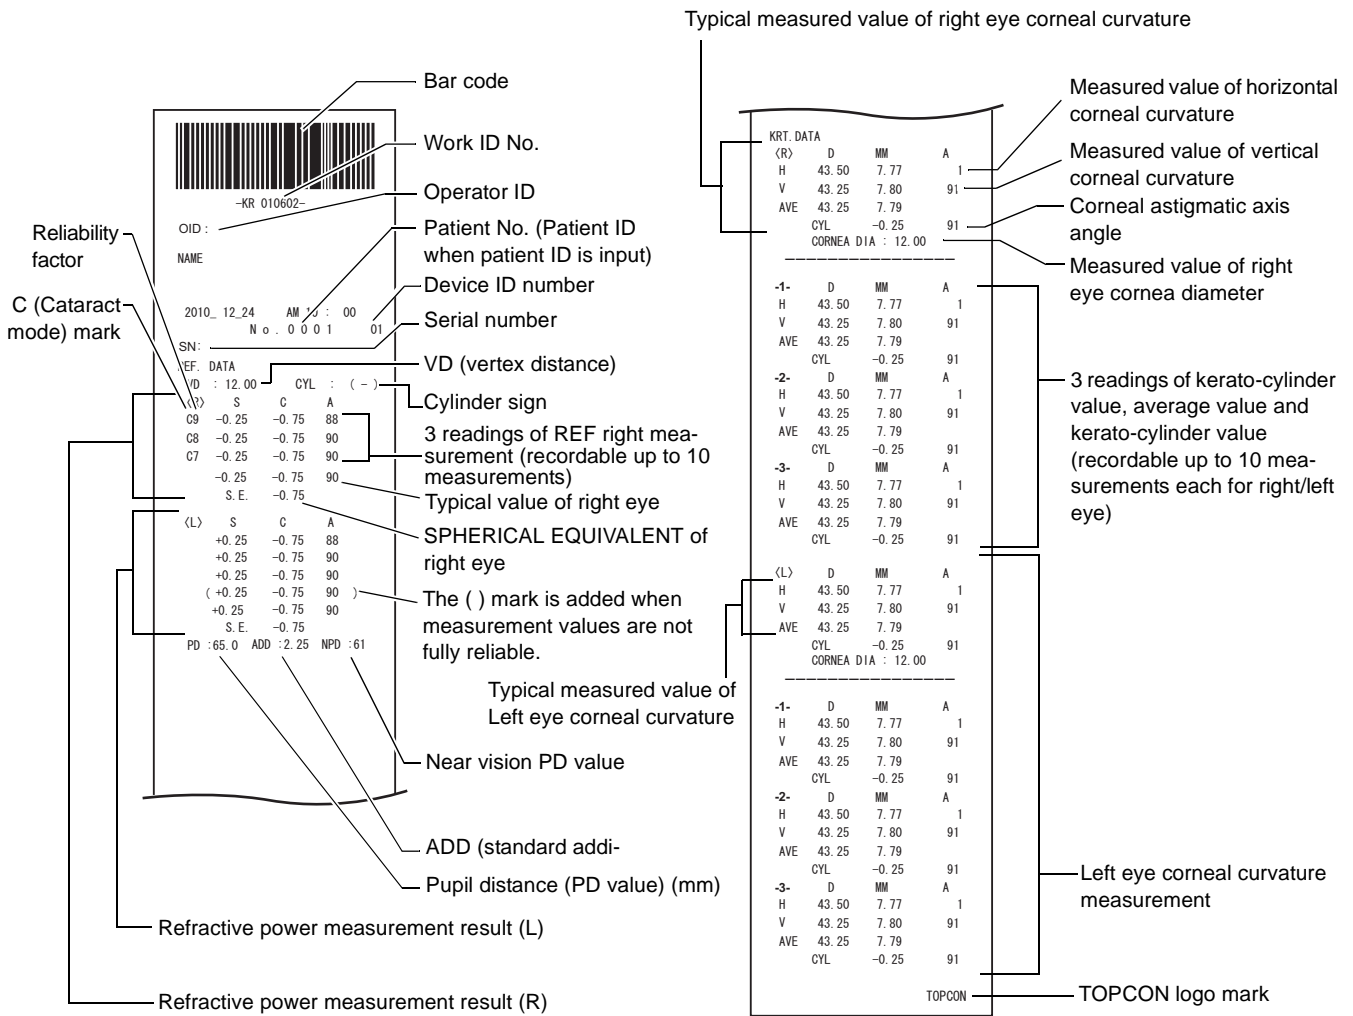



**NOTE**

- The reliability factor is defined with integers 1 to 9 in increasing order of reliability. Additionally, if the reliability is high enough, the reliability factor is not shown on the printout.
- The Near PD value is calculated based on the ADD.
- ( ) appears when normal measurement is not expected due to eyelid, eyelash, or blinking.
- \*-mark appears when normal measurement is not expected with the Cataract button selected.

KRT typical value style and KRT print data are R1R2

Barcode

Work ID No. -KR 010602-

Operator ID

Reliability factor

C (Cataract mode) mark

Patient No. (Patient ID when patient ID is input)

Device ID number

Serial number

VD (vertex distance)

REF. DATA

VD : 12.00 CYL : ( - )

Cylinder sign

Result of refractory power measurement (Right eye)

3 readings of REF right measurement (recordable up to 10 measurements)

Typical value of right eye

Spherical equivalent of right eye

The ( ) mark is added when measurement values are not fully reliable.

Result of refractory power measurement (Left eye)

Near vision PD value

ADD (ordinary additional power)

Pupil distance (PD value) (mm)

KRT DATA

Measured value of flat meridian corneal curvature

Measured value of steep meridian corneal curvature

D: Average value of corneal refractive power

MM: Average value of cornea curvature radius

KRT data (Right eye)

Corneal astigmatic axial angle

Measured value of right eye cornea diameter (mm)

KRT data (Left eye)

MM1: Corneal refractive power at flat meridian

MM2: Corneal refractive power at steep meridian

A1: Angle of flat meridian

\*-mark appears when reliability of the measurement is too low.

**NOTE**

- The reliability factor is defined with integers 1 to 9 in increasing order of reliability. Additionally, if the reliability is high enough, the reliability factor is not shown on the printout.
- The Near PD value is calculated based on the ADD.
- ( ) appears when normal measurement is not expected due to eyelid, eyelash, or blinking.
- \*-mark appears when normal measurement is not expected with the Cataract button selected.

## PRINTOUT FORMAT SETTING

Printout format can be changed by pushing "Print" in the Settings screen. For Print settings, see "SETTING FUNCTIONS ON SETUP SCREEN" on page 42.

### PRESET

All: Initial setting (all measurement values are printed.)

Ave: Only average values are printed.







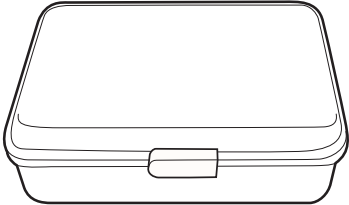



Classic: Equivalent with RM/KR-8900 Classic 2

	ITEM	INITIAL	PRESET		
			All	Ave	Classic*
Common	Barcode	OFF	OFF	OFF	OFF
	Operator ID	OFF	OFF	OFF	OFF
	Name	ON	ON	ON	ON
	Date	ON	ON	ON	ON
	Date style	MDY	MDY	MDY	MDY
	Patient No./Patient ID	ON	ON	ON	ON
	Device ID	OFF	OFF	OFF	OFF
	Serial number	ON	ON	ON	ON
	Include error data	OFF	OFF	OFF	OFF
	TOPCON logo	ON	ON	ON	ON
	Message print	OFF	OFF	OFF	OFF
	Input message	NULL	NULL	NULL	NULL
	Graphic print	Normal Printer	Normal Printer	Normal Printer	Normal Printer
	Line space	0	0	0	0
	Auto Cut	ON	ON	ON	ON
REF/KRT*	Print Layout	DATA	DATA	DATA	DATA
	VD	ON	ON	ON	ON
	Cylinder sign	ON	ON	ON	ON
	Print form of REF result	ALL	ALL	AVE	ALL
	Reliability	OFF	OFF	OFF	OFF
	S.E.	ON	ON	ON	ON
	PD	ON	ON	ON	ON
	ADD	OFF	OFF	OFF	OFF
	KRT print layout	D/mm	D/mm	D/mm	D/mm
	Print form of KRT result	ALL	ALL	AVE	AVE
	KRT ave. -HV or R1R2	R1R2	R1R2	R1R2	HV
	KRT data -HV or R1R2	R1R2	R1R2	R1R2	HV
	KRT average	ON	ON	ON	ON
KRT cylinder	ON	ON	ON	ON	
Cornea diameter	ON	ON	ON	ON	
REF	VD	ON	ON	ON	ON
	Cylinder sign	ON	ON	ON	ON
	Print form of REF result	ALL	ALL	AVE	ALL
	Reliability	OFF	OFF	OFF	OFF
	S.E.	ON	ON	ON	ON
	PD	ON	ON	ON	ON
	ADD	OFF	OFF	OFF	OFF
KRT*	KRT print layout	D/mm	D/mm	D/mm	D/mm
	Print form of KRT result	ALL	ALL	AVE	ALL
	KRT ave. -HV or R1R2	R1R2	R1R2	R1R2	HV
	KRT data -HV or R1R2	R1R2	R1R2	R1R2	HV
	KRT average	ON	ON	ON	ON
	KRT cylinder	ON	ON	ON	ON
Cornea diameter	ON	ON	ON	ON	

\* : Only in KR-800


## **STANDARD ACCESSORIES**

The following are standard accessories. Make sure that all these items are included (quantity).


<p>Power cable (1)</p> 	<p>Chinrest tissue pin (2)</p> 
<p>Printer paper (2)</p> 	<p>Monitor cleaner (1)</p> 
<p>Chinrest tissue (1)</p> 	<p>Dust cover (1)</p> 
<p>Accessory case (1)</p> 	<p>User manual, Unpacking and Assembling (1 each)</p> 
<p>Rubber cap (1)</p> 	<p>Model eye (1)</p> 

# PREPARATIONS



## INSTALLATION

 <b>CAUTION</b>	<ul style="list-style-type: none"><li>• When moving the instrument, two people should lift from the bottom of the device. One person lifting the device may cause harm to his back or injury by falling parts. Also, holding areas other than the bottom and holding the External I/O terminal cover may cause injury, as well as damage to the instrument.</li><li>• To prevent damage and injuries, do not install the instrument on an uneven, unsteady or sloped surface.</li><li>• When setting an instrument on an instrument table, pay attention not to injure the patient's fingers between the instrument and the table.</li></ul>
--	--

- 1** Use the base stopper to fix the main body.
- 2** Firmly hold the instrument at the position shown below and place it on the automatic instrument table. For the adjustable instrument table, see "OPTIONAL ACCESSORIES" on page 69.

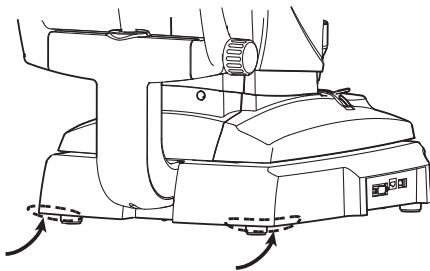


Holding positions

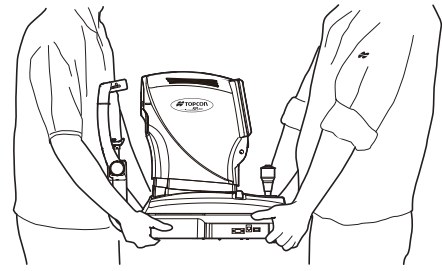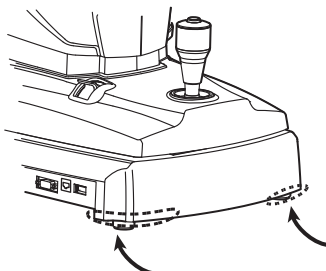


Holding the instrument


- 3** After installation, turn the base stopper down. The main body can be moved.

## CONNECTING POWER CABLE

 <b>WARNING</b>	<p>Be sure to connect the power plug to an AC 3-pin receptacle equipped with grounding. Connection with receptacle without grounding may cause fire and electric shock in case of short-circuiting.</p>
--	---

 <b>CAUTION</b>	<p>To avoid electric shocks, do not handle the power plug with wet fingers.</p>
--	---

- 1** Make sure the POWER switch of the instrument is OFF.
- 2** Connect the power cable to the power inlet at the right side of the instrument.
- 3** Insert the power cable plug into the 3-pin AC grounding receptacle.

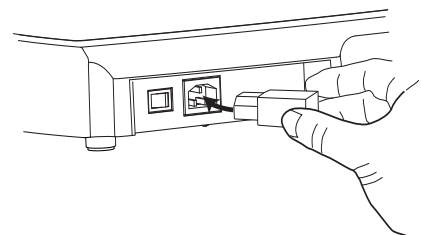

## CONNECTING EXTERNAL I/O TERMINALS



### CAUTION

To avoid electric shock, do not touch the external connection terminal and the patient at the same time.




### NOTE

When connecting this product with a commercial personal computer, use one conforming to IEC60950/IEC60950-1, with a separation unit.

## DATA OUTPUT

This product can be connected to a personal computer (PC) and other external devices via the RS-232C or LAN.

- 1** Connect the connection cable to the output terminal of the instrument
- 2** Connect the other end of the connection cable to the PC, etc.

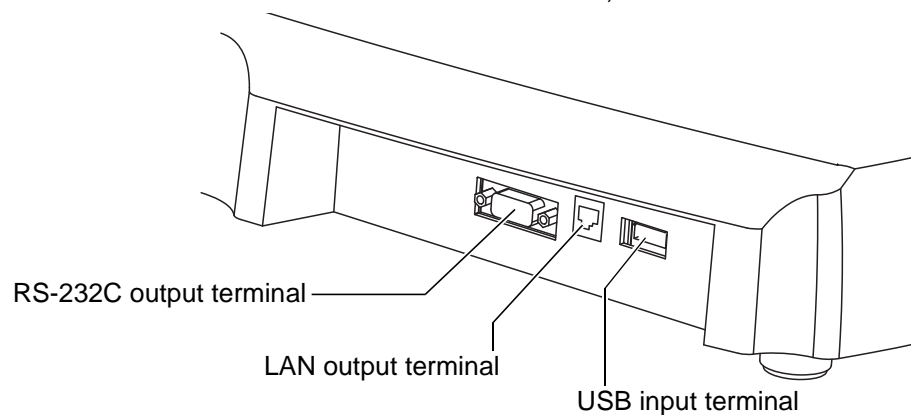

## DATA INPUT

This product can be connected to a bar-code reader and other external devices via USB.

- 1** Connect the connection cable to the input terminal of the instrument.
- 2** Connect the other end of the connection cable to the external device.



### NOTE

For questions about connections, contact your TOPCON dealer.

## PRINTER PAPER SETTING



### CAUTION


- To avoid failure or potential injury, do not open the printer cover while the printer is in operation.
- To avoid potential injury in case of malfunction, including a paper jam, be sure to shut off the power before attempting to repair it.
- To avoid potential injury, do not touch the printer body including metal parts or the paper cutter, while the printer is in operation or when replacing the printer paper.
- Pay much attention not to touch the internal printer's body when the cover is open. If touched, it may result in trouble due to electrostatic discharge.
- When pressing the printer cover open switch, be careful that the instrument does not touch the patient's lip or nose. If touched, clean the instrument following "CLEANING THE FOREHEAD REST AND CHIN REST" on page 52.




### NOTE

- If you insert the printer paper backwards, printing will not start.
- Please push the printer cover OPEN switch using your right thumb while placing your index and middle fingers on the projecting part which is in reverse side below the switch. Unexpected movement is avoided when the printer cover OPEN switch is pressed.


**1** Press the printer cover open switch to open the printer cover.

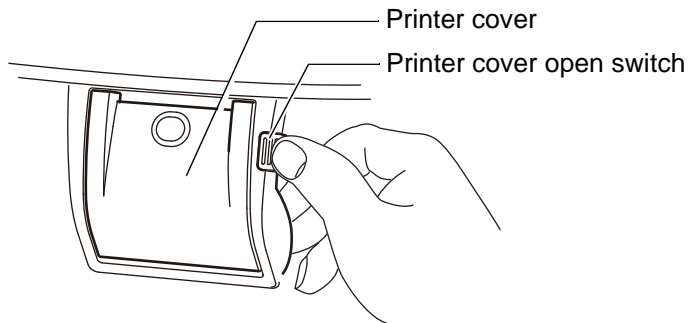

**2** Open the printer cover to the limit.




**3** Insert the printer paper in the direction shown below and pull out the paper end to your side by 7 to 8cm.

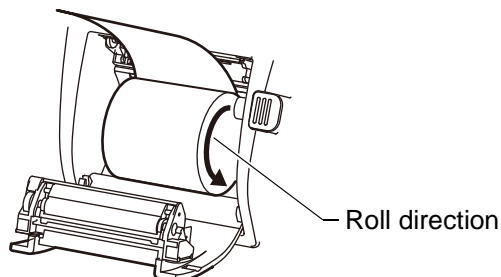



- 4 Bring the paper into the center, then close the printer cover.



## NOTE

- Please close the printer cover using your right thumb while placing your index and middle fingers on the projecting part which is in reverse side below the printer cover OPEN switch. Unexpected movement is avoided when closing the printer cover.
- In case the printer cover is not firmly closed, printing will not start, and "CLOSE PRT COVER" will be displayed on the monitor screen.
- A 58mm wide paper roll (example: TP-50KJ-R [Nippon Paper Co.]) is recommended.  
Other paper rolls may cause abnormal printing noise or unclear print.

## RECOVERY FROM POWER SAVE STATUS

This instrument adopts the power save system for saving electric power. When the machine is not operated for a set time, the control panel becomes a screensaver.

- 1 Tap the control panel or operate the control lever.

In a few seconds, the measurement screen is displayed and measurement is enabled.



## NOTE

The time to start the power save status can be changed in the initial setting "Start time of sleep mode" (see page 46).

# BASIC OPERATIONS

## PREPARATION BEFORE MEASUREMENT

### TURNING ON THE INSTRUMENT


- 1** Make sure the power cable is connected properly.  
For the details of connection, refer to "CONNECTING POWER CABLE" on page 20.
- 2** Press on the **POWER** switch.
- 3** Make sure that the title screen is displayed and then the MEASUREMENT screen is displayed in a few seconds.

### SELECTING THE MEASUREMENT MODE (ONLY IN KR-800)

This product has three measurement modes: R/K (REF/KRT continuous measurement), KRT (KRT single measurement) and REF (REF single measurement).

- 1** Check that the MEASUREMENT screen is on.
- 2** Tap the **MEASUREMENT MODE** button on the control panel and select the measurement mode. Indication of the **MEASUREMENT MODE** button is changed.

REF: Only REF measurement  
KRT: Only KRT measurement  
R/K: REF/KRT continuous measurement

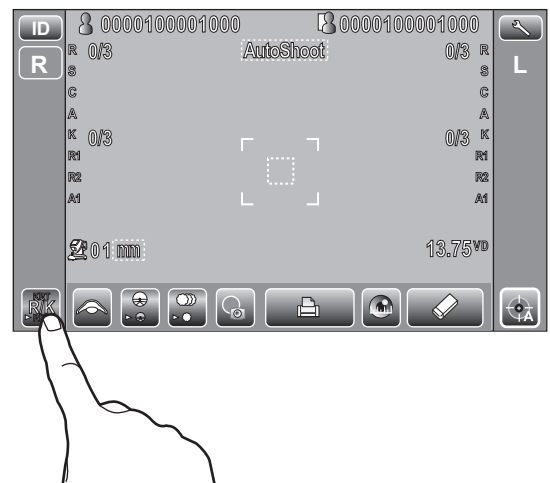

## PATIENT POSITIONING



### CAUTION


- To avoid electric shock, do not touch the external connection terminal and the patient at the same time.
- To avoid injury, do not insert fingers under the chinrest. To avoid injury when moving the chinrest down, be careful not to catch the patient's finger. Tell this to the patient, too.
- To avoid injury when operating the machine (for measurement and control panel operation), be careful about the cover not to catch fingers of the patient. Tell this to the patient, too.
- To avoid injury by raising, falling or dropping the instrument, do not apply the strong power downward on the chinrest.
- When operating the instrument (for measurement and control panel operation), be careful that the instrument does not touch the patient's lip or nose. If touched, clean the instrument following "CLEANING THE FOREHEAD REST AND CHIN REST" on page 52.




### NOTE

- Adjust the height of the adjustable instrument table so that the patient can sit on the chair comfortably. Otherwise, correct measurement values may not be obtained.

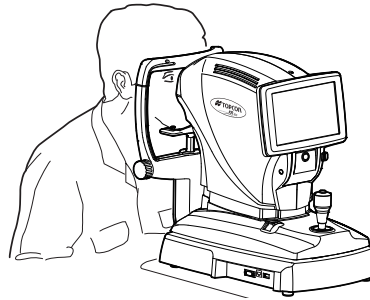

- 1** Check the measurement screen.
- 2** Have the patient sit in front of the instrument.
- 3** Adjust the adjustable instrument table or the chair height for the patient to put his/her chin on the chinrest comfortably.
- 4** Place the patient's chin on the chinrest and check that his/her forehead is touching to the forehead rest.

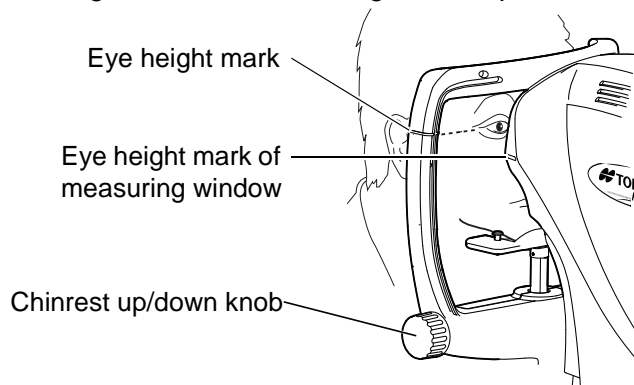

- 5** Adjust the chinrest height by chinrest up/down knob until the eye height mark of the chinrest reaches the same height as the patient's eye. At this moment, confirm that the height mark of the measuring window is at the height of the patient's visual line.




## AUTO SHOOT MODE MEASUREMENT (ONLY IN KR-800)

 <b>CAUTION</b>	When operating the instrument (for measurement and control panel operation), be careful that the instrument does not touch the patient's lip or nose. If touched, clean the instrument as specified in "CLEANING THE INSTRUMENT" on page 52.
 <b>NOTE</b>	<ul style="list-style-type: none"><li>• Auto Shoot mode measurement may not be possible, in case the eyelid and the eyelashes cover the pupil. If this occurs, the operator should tell the patient to open their eyes as wide as possible, or lift the eyelid to allow for measurement.</li><li>• Auto Shoot mode measurement may not be possible due to frequent blinks or existing abnormalities in the corneal surface caused corneal disease etc. In this case, select manual mode.</li></ul>

## SETTING THE AUTO SHOOT MODE


- 1** Check the measurement screen. If **Auto Shoot** button is framed in orange, it is in Auto Shoot mode.
- 2** If **Auto Shoot** button is not framed in orange, it is in manual mode. Tap the Auto Shoot button to change to Auto Shoot mode.

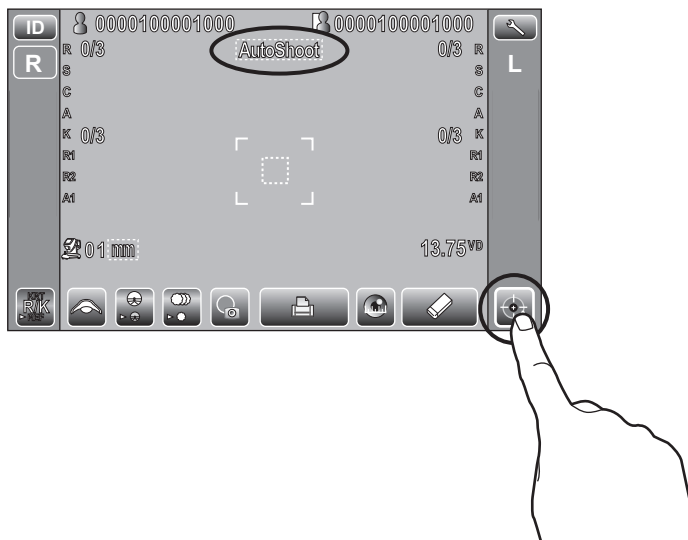

## ALIGNMENT AND MEASUREMENT


Alignment operations are done with the control lever.

- The main body position can be fine-adjusted laterally by inclining the control lever to each direction.

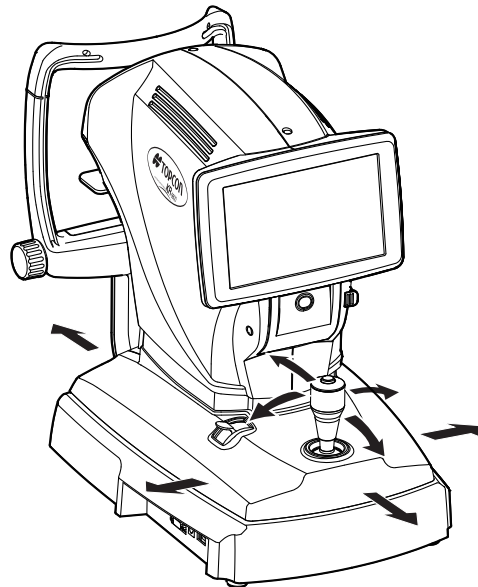

Operating the control lever  
(for lateral adjustment)

- The main body position can be fine-adjusted vertically by turning the control lever right (up) and left (down).

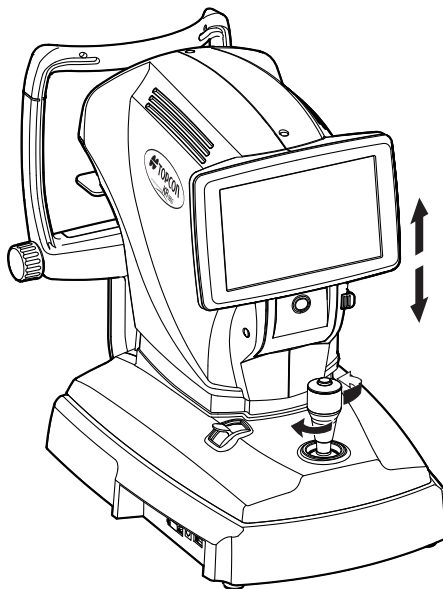


Operating the control lever  
(for up/down adjustment)




### NOTE

If Auto Shoot mode measurement does not work, select manual mode.  
Auto Shoot mode measurement may not work depending on the cornea condition.


- 1 Use the base stopper to release the main body.  
Hold the control lever and move the main body to the operator side.

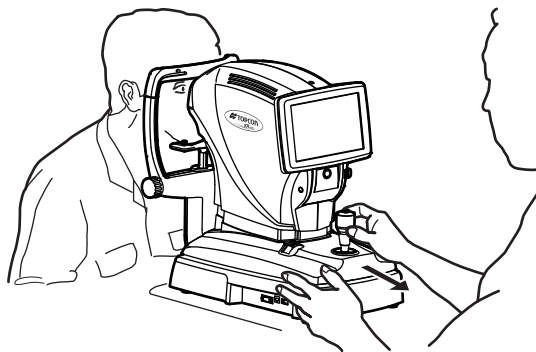


- 2 Operate the control lever laterally and vertically to obtain the target eye in the center of control panel screen.

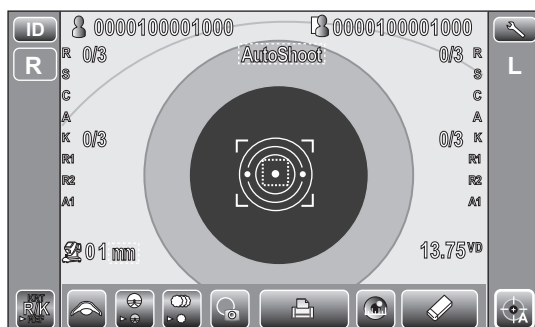

- 3 While moving the main body toward the patient, focus the target eye.  
A vague, reflected alignment dot appears on the cornea.

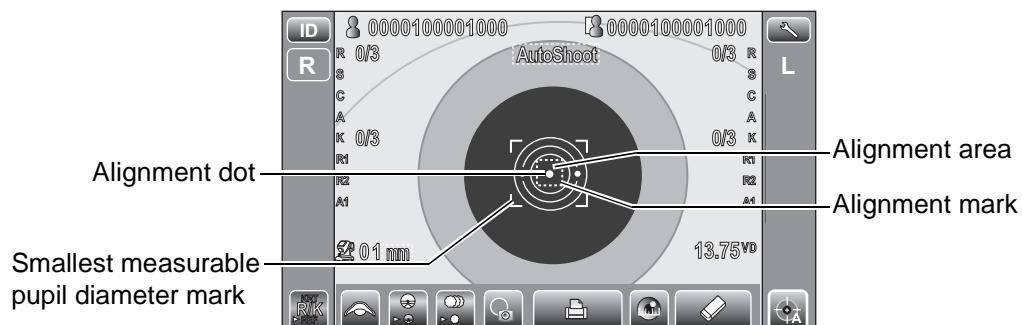


- 4 Fine-adjust the main body position in all directions so that the alignment dot point comes within the alignment area.
- 5 Keeping the alignment dot within the alignment area, slowly move the main body toward the patient. When the main body approaches the target eye, alignment arrows appear to the control panel screen.


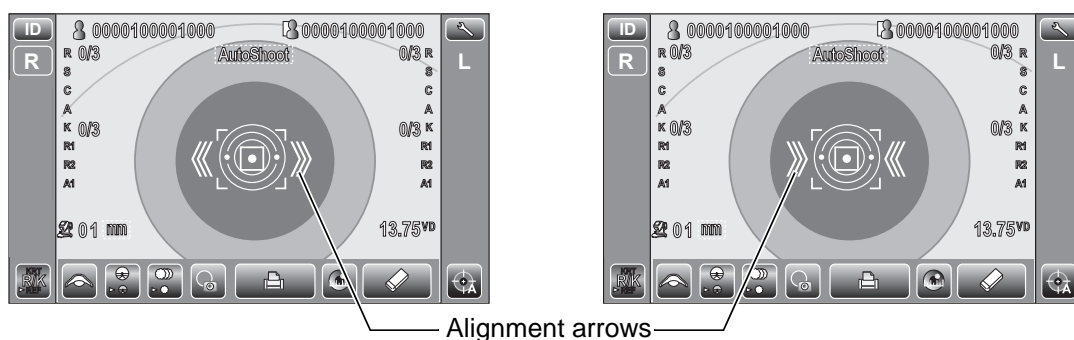


**NOTE**



- Do not allow the eyelash and eyelid to cover the smallest measurable pupil diameter mark to ensure stable measurement.
- If the machine is too near to the patient in comparison with the optimal alignment position, the alignment arrows are displayed outward. If it is too far from the patient, the alignment arrows are displayed inward.




Too close

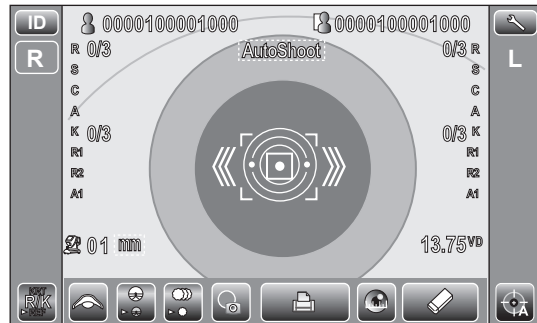

Too far

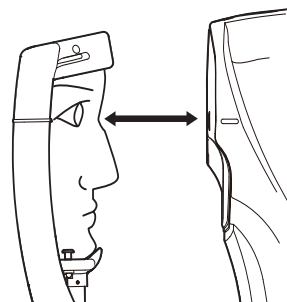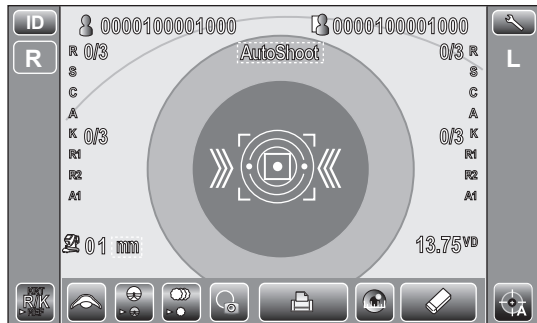


Positioning is incorrect at all.

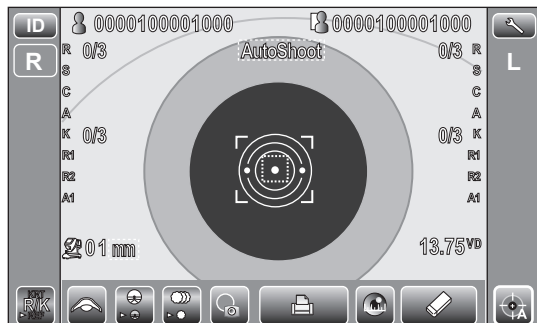


**NOTE**

When the measuring head has reached the limit of movement (vertical/lateral directions), a yellow-colored limit mark appears on the control panel's top, showing it is the movement limit in that direction. Move the measuring head or chinrest to a position that aligning is possible.

Limit mark

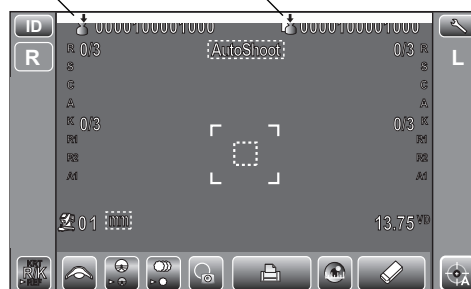

- 6** After the alignment arrows are displayed, move the main body slowly towards the patient. Measurement is done and the measurement value is displayed on the monitor screen.

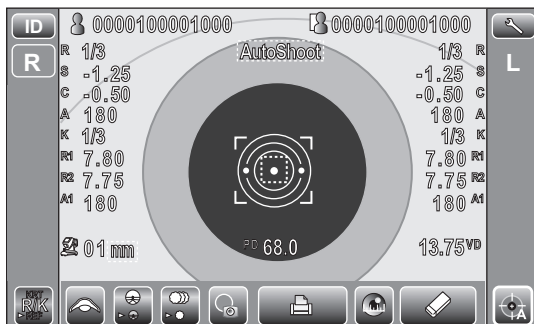

 **NOTE**

- If Auto Shoot mode measurement does not work, select manual mode. Auto Shoot mode measurement may not work depending on the cornea condition.
- If the machine is moved before measurement values are displayed, it might cause an incorrect measurement.
- Auto print (available only under Auto Shoot mode)  
When auto print setting is "ON" in the initial setting, the buzzer sounds twice after measuring the right and left eyes, and measurement results are printed out automatically.
- When auto print setting is "OFF" in the initial setting, print out measurement results by tapping the Print button, as necessary. (Only in KR-800)

## DISPLAYING MEASUREMENT VALUES

Data of the latest measurement are displayed on the control panel screen.

Figures only: Measurement was done correctly.

ERROR: Measurement was not done correctly.

 **NOTE**


For explanation of the messages on the control panel screen, refer to "MESSAGE LIST" on page 57.



## **MANUAL MODE MEASUREMENT**

### **SETTING THE MANUAL MODE (ONLY IN KR-800)**

- 1** Check the measurement screen. If **Auto Shoot** button is not framed in orange, it is in Manual mode.
- 2** If **Auto Shoot** button is framed in orange, it is in Auto Shoot mode. Tap the **Auto Shoot** button to change to manual mode.

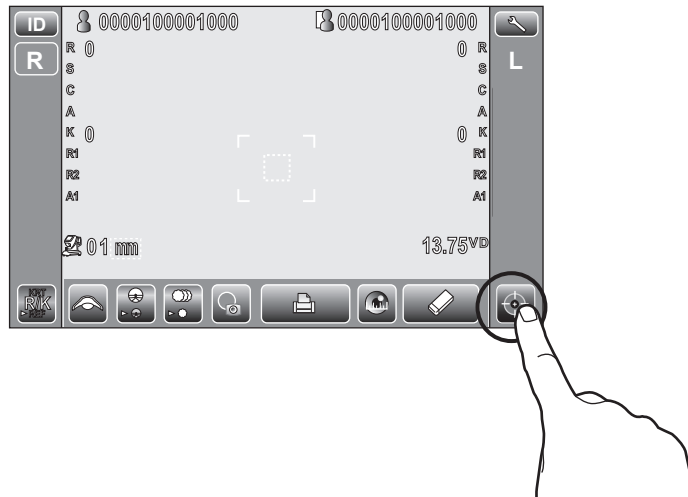


### **ALIGNMENT AND MEASUREMENT**

Alignment is operated on the control panel.

For the adjustment of main body using the control lever, refer to page 27.

- 1** Use the base stopper to release the main body.  
Hold the control lever and move the main body to the operator side.

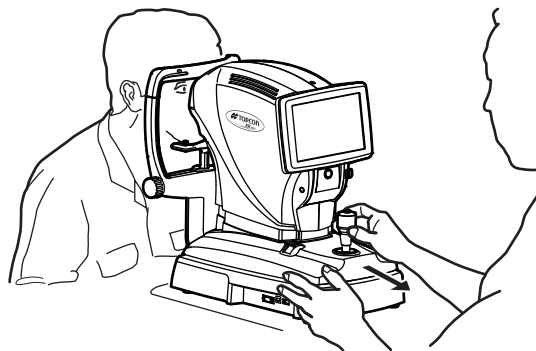

- 2** Operate the control lever laterally and vertically to obtain the target eye in the center of monitor screen.




#### **NOTE**

If the pupil is not displayed on the control panel, move the measuring head, checking the eye height mark on the measurement window as a guide (see page 25).

**NOTE**


When the measuring head has reached the limit of movement (vertical/lateral directions), a yellow-colored limit mark appears on the control panel's top, showing it is the movement limit in that direction. Move the measuring head or chinrest to a position that aligning is possible.

Limit mark

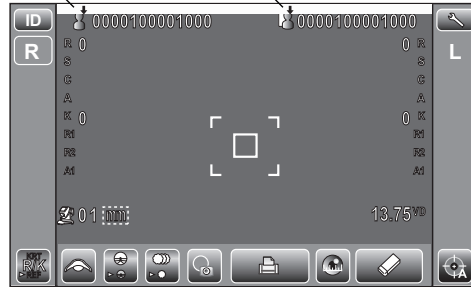

**3** While moving the main body toward the patient, focus the target eye.

A vague, reflected alignment dot appears on the cornea.

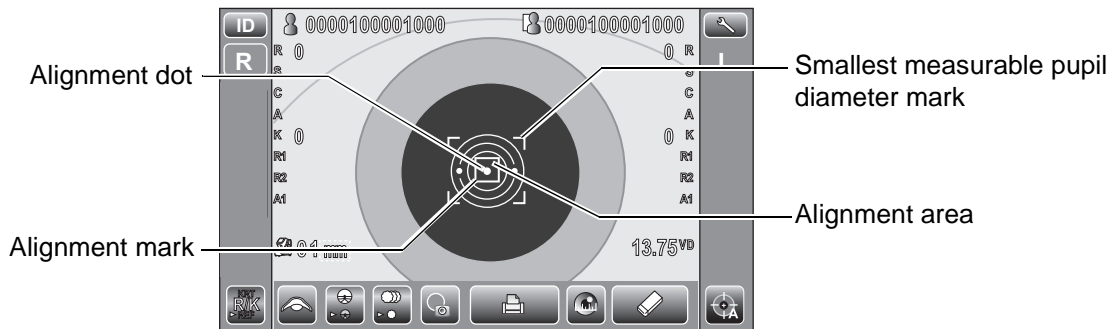


**4** When the alignment dot becomes the minimum within the alignment area, press the

**MEASUREMENT switch**.

**NOTE**

- Do not allow the eyelash and eyelid to cover the smallest measurable pupil diameter mark to ensure stable measurement.
- Even if fine alignment has not been achieved, measurement can be performed by pressing the **MEASUREMENT switch**. To ensure correct measurement, try to get fine alignment.

**5** Measurement is performed and measurement values are displayed on the control panel.

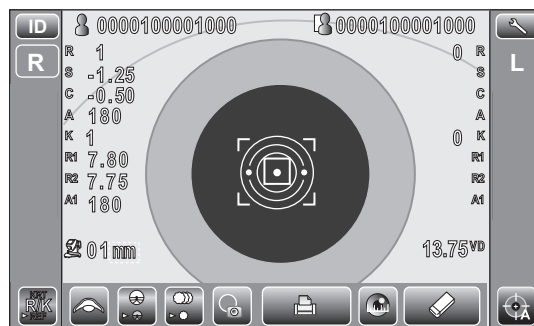

**NOTE**

If the machine is moved before measurement values are displayed, it may cause incorrect measurement result.

## DISPLAYING MEASUREMENT VALUES

Data of the latest measurement are displayed on the control panel screen.

Figures only: Measurement was done correctly.

ERROR: Measurement was not done correctly.



### NOTE

For explanation of the messages on the control panel screen, refer to "MESSAGE LIST" on page 57.

## PRINT-OUT OF MEASUREMENT VALUES



### NOTE

- To avoid a paper jam in the printer, do not feed the paper if it is partly cut or wrinkled.
- To avoid discoloring of the printer paper (particularly the recording area) during storage, use a polypropylene bag and not one containing plasticizer (PVC, etc.).
- To avoid discoloring of the printer paper (particularly the recording area) after pasting, use water-soluble glue and not one containing solvent.
- Since the printer paper is thermosensitive, it is not suitable for keeping records for a long period. If necessary, prepare copies separately.


This instrument can print out measurement values by a printer.

**1** Check the Measurement screen is on.

**2** Tap the  button on the control panel.

Measurement values on the monitor are printed out.

After being printed out, the measurement values on the screen are deleted automatically.

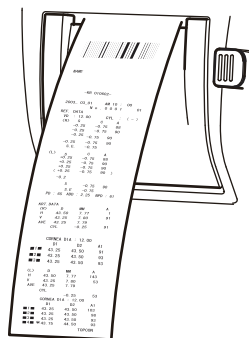


## NOTE

- When the cylindrical refractive power is "0," the direction of astigmatic axis and measurement values are not displayed/printed.
- When a red line is printed at the end of the printer paper, replace it with a new one. For details about the replacement of printer paper, see "PRINTER PAPER SETTING" on page 22. 58mm wide printer paper (example: TP-50KJ-R, Nippon Paper) is recommended.
- "CLOSE PRT COVER" is indicating that the printer cover is left opened, ensure that the printer cover is completely closed.
- When auto print is setting is "ON" in the initial setting, measurement is performed under Auto mode, and measurement results are printed out automatically. (See page 46. Only in KR-800)
- When the Auto cut setting is off and you need to cut a printer form, the way is that erase the measurement value by tapping the **ALL CLEAR** button, and tap the **PRINT OUT** button. (See page 48.)

## CLEARING MEASUREMENT VALUES

- 1 Tap the **ALL CLEAR** button on the control panel.  
All measurement values of both eyes are cleared.

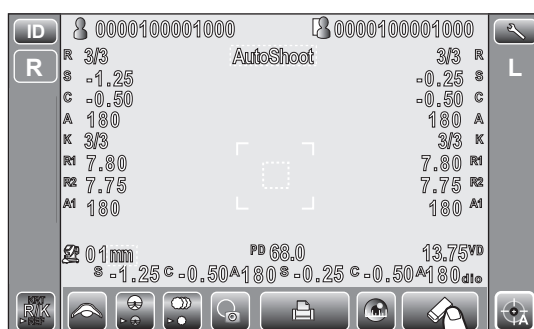


# DISPLAYING ALL MEASUREMENT DATA


Normally the latest measurement is displayed, but it is possible to display and confirm all measurement data.

Measurement data chooses and displays "REF data" and "KRT data (Only in KR-800)."

**1** Tap the **TARGET IMAGE** button of the control panel.

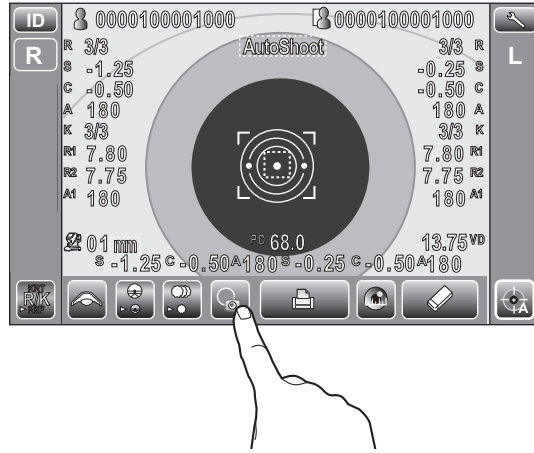

**2** Tap the **ALL DATA DISPLAY** button.

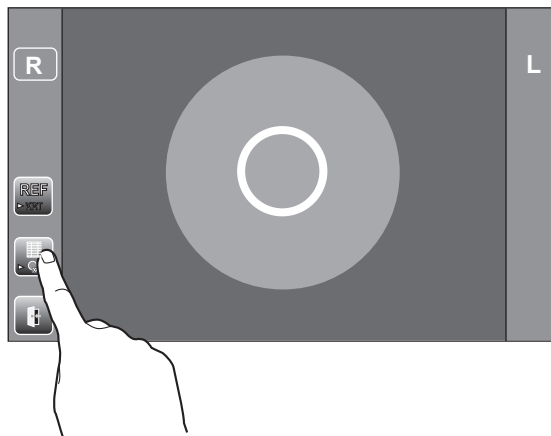

**3** The Data Display screen is displayed.

RIGHT				LEFT			
	S	C	A		S	C	A
C1	-1.25	-0.50	180	1	-0.25	-0.50	180
2	-1.25	-0.50	180	2	-0.25	-0.50	180
(3)	-1.25	-0.50	180	3	-0.25	-0.50	180
4				4			
5				5			
6				6			
7				7			
8				8			
9				9			
10				10			
AVE	-1.25	-0.50	180	AVE	-0.25	-0.50	180

When measurement is performed with the Cataract button ON, "C" comes at the head of figures.

When Cataract mode starts automatically during the measurement, figures will be put in ( ).

RIGHT				LEFT			
	S	C	A		S	C	A
C1	-1.25	-0.50	180	1	-0.25	-0.50	180
2	-1.25	-0.50	180	2	-0.25	-0.50	180
(3)	-1.25	-0.50	180	3	-0.25	-0.50	180
4				4			
5				5			



## NOTE

When no data is memorized, the data table shows blank.

- 4** To change "REF data" and "KRT data (Only in KR-800)," tap the **REF/KRT** button.

RIGHT				LEFT			
	R1	R2	A1		R1	R2	A1
1	7.80	7.75	180	1	7.80	7.75	180
2*	7.80	7.75	180	2	7.80	7.75	180
3*	7.80	7.75	180	3	7.80	7.75	180
4				4			
5				5			
6				6			
7				7			
8				8			
9				9			
10				10			
AVE	7.80	7.75	180	AVE	7.80	7.75	180

When the reliability of KRT data is low, "\*" is attached after the figures.

RIGHT				LEFT			
	R1	R2	A1		R1	R2	A1
1	7.80	7.75	180	1	7.80	7.75	180
2*	7.80	7.75	180	2	7.80	7.75	180
3*	7.80	7.75	180	3	7.80	7.75	180
4				4			

- 5** To exit the data display and return to the Measurement screen, tap the **EXIT** button.

RIGHT				LEFT			
	R1	R2	A1		R1	R2	A1
1	7.80	7.75	180	1	7.80	7.75	180
2*	7.80	7.75	180	2	7.80	7.75	180
3*	7.80	7.75	180	3	7.80	7.75	180
4				4			
5				5			
6				6			
7				7			
8				8			
9				9			
10				10			
AVE	7.80	7.75	180	AVE	7.80	7.75	180

## OPERATION OF AFTER USE

- 1** Use the base stopper to fix the main body.
- 2** Turn the POWER switch to off.



## NOTE

When external devices are connected to external I/O terminals, turn off the power of these devices too.  
(If power switch is provided.)

- 3** Unplug the power cable from a 3-pin AC inlet with grounding.



## NOTE

When the instrument is not used for a long period, unplug the power supply cable, and detach the cable connected to the external I/O terminal.

# OPTIONAL OPERATIONS

## DISPLAYING THE PATIENT ID (PATIENT No.) OR OPERATOR ID

A patient ID or operator ID of up to 13 characters can be input and displayed on the control panel and printout.

However, if no patient ID is input, the patient No. is allocated automatically by the device.

**1** Tap  button.

**2** Tap keyboard on the screen and enter characters. Tap  button and fix the input value.



### NOTE

Patient ID is reset when measurement values are printed or if the  button is tapped.


Patient No. reset condition can be selected such that the patient No. is reset upon power on or not, in the initial setting of setup screen.

"Refer to "Patient No. reset" on page 46.


# MEASUREMENT OF CORNEA DIAMETER (ONLY IN KR-800)

## MEASUREMENT ON THE ACTUAL IMAGE


- 1 Tap the **CORNEA DIAMETER** button.

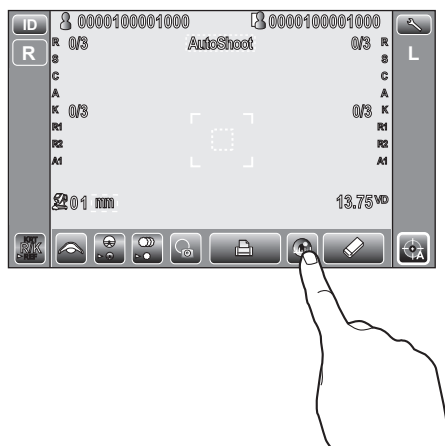

- 2 The Cornea Diameter Measurement screen is displayed, and the positioning bar is displayed.

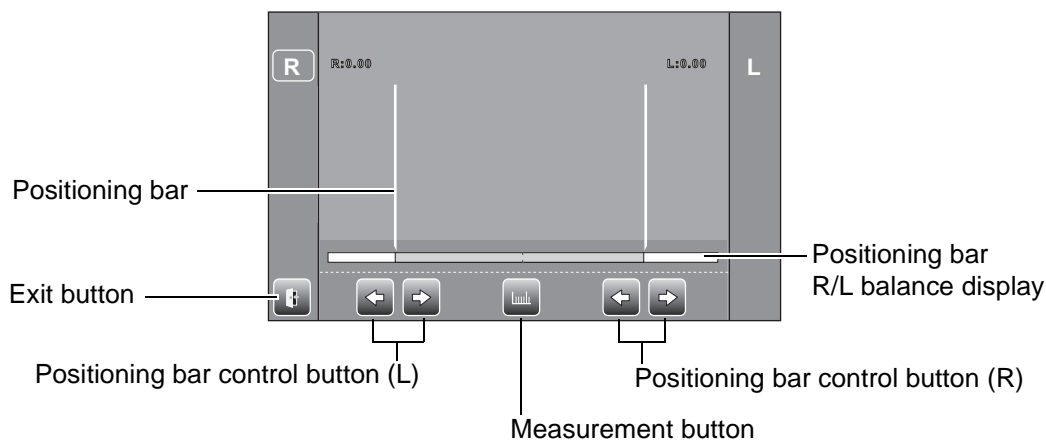


- 3 When the pupil is displayed, moves the measuring head so that the pupil image and alignment dot are at the center of the screen.
- 4 Using the **POSITIONING BAR CONTROL** button (L), move the left positioning bar to the left end of the iris from the control panel side.

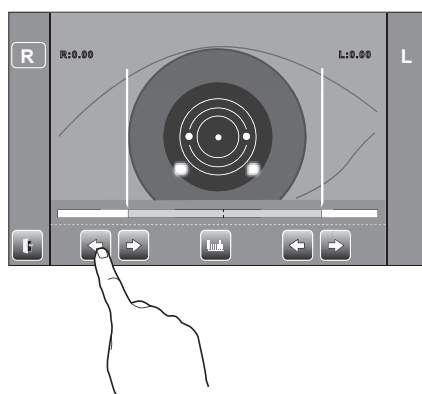



- 5 Using the **POSITIONING BAR CONTROL** button (R), move the right positioning bar to the right end of the iris from the control panel side.

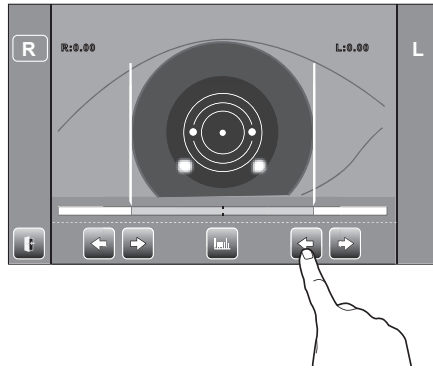


## NOTE

By tapping the positioning bar R/L balance display, positioning bar can be moved.

- 6 Tap the **MEASUREMENT** button.

- 7 The cornea diameter is displayed.

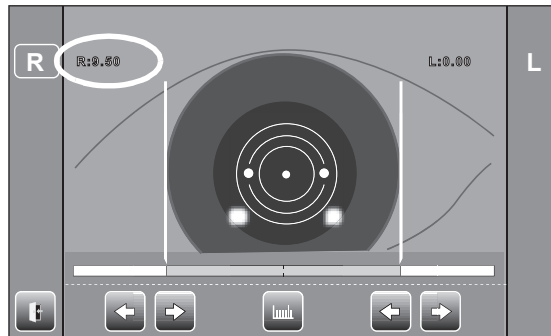


- 8 Move the measuring head to the other eye measurement position. In like manner, measure the other eye.

- 9 Tap the **EXIT** button and return to the Measurement screen.


## MEASUREMENT ON THE STILL IMAGE

When KRT measurement values are available, the still image of the measurement is displayed.


- 1 Follow steps 1 to 3 of "MEASUREMENT ON THE ACTUAL IMAGE" and display the cornea image at the screen center.
- 2 Press the  to display the saved image.

 <b>NOTE</b>	If you are required to get the still image again, press the <input type="button" value="MEASUREMENT switch"/> to return to actual image, and press the <input type="button" value="MEASUREMENT switch"/> again.
---	---

- 3 Tap either of the (R)/(L)  buttons and move the positioning bar.

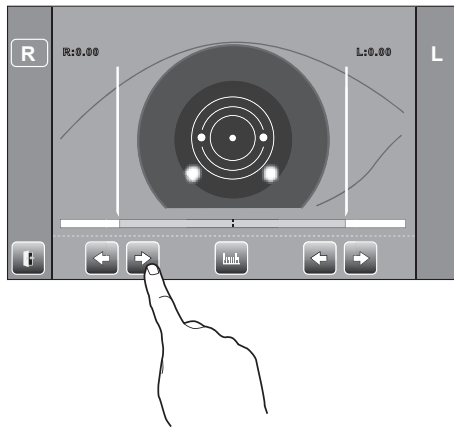

- 4 Follow steps 4 to 6 of "MEASUREMENT ON THE ACTUAL IMAGE."
- 5 The cornea diameter is displayed.

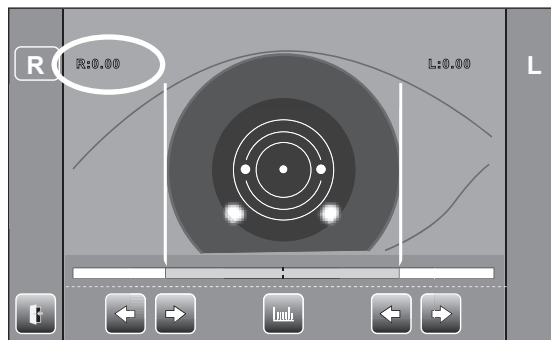

- 6 Move the measuring head to the other eye measurement position.  
In like manner, measure the other eye.
- 7 Tap the  button and return to the Measurement screen.

## **OUTPUT USING RS-232C**

This instrument can output data to a PC, etc. via the RS-232C interface.

- 1** Connect the interface cable to RS-232C OUT.  
Refer to "CONNECTING EXTERNAL I/O TERMINALS" on page 21.
- 2** Set up of data communication settings.  
For details, refer to "DATA COMMUNICATION (COMM)" on page 50.
- 3** Perform measurements.
- 4** Tap the **PRINT OUT** button of the control panel.  
When output is completed, "RS-232C SUCCESS" is displayed on the screen.

## **INPUT USING USB**

This instrument can input ID numbers from a bar code reader, etc. via the USB.

- 1** Check the connection of USB IN.  
For connection, refer to "CONNECTING EXTERNAL I/O TERMINALS" on page 21.
- 2** Input ID numbers from the external device.  
The inputted ID numbers are displayed on the screen.

## **OUTPUT USING LAN**

This instrument can output data to a PC, etc. via the LAN interface.

- 1** Connect the network cable to LAN OUT.  
For connection, refer to "CONNECTING EXTERNAL I/O TERMINALS" on page 21.
- 2** Set up of LAN connection settings.  
For details, refer to "LAN CONNECTION (LAN)" on page 51.
- 3** Perform measurements.
- 4** Tap the **PRINT OUT** button of the control panel.  
When output is completed, "LAN SUCCESS" is displayed on the screen.



### **NOTE**

For explanation of messages during communication refer to the "MESSAGE LIST" on page 57.


# SETTING FUNCTIONS ON SETUP SCREEN

## OPERATING THE SETUP SCREEN


Various functions can be set on the SETUP screen.

### PREPARATIONS FOR SETTING

- 1 Make sure that the power cable is connected.  
For connection, refer to "CONNECTING POWER CABLE" on page 20.
- 2 Turn ON the **POWER** switch.
- 3 Tap the **SETTINGS** button on the control panel.

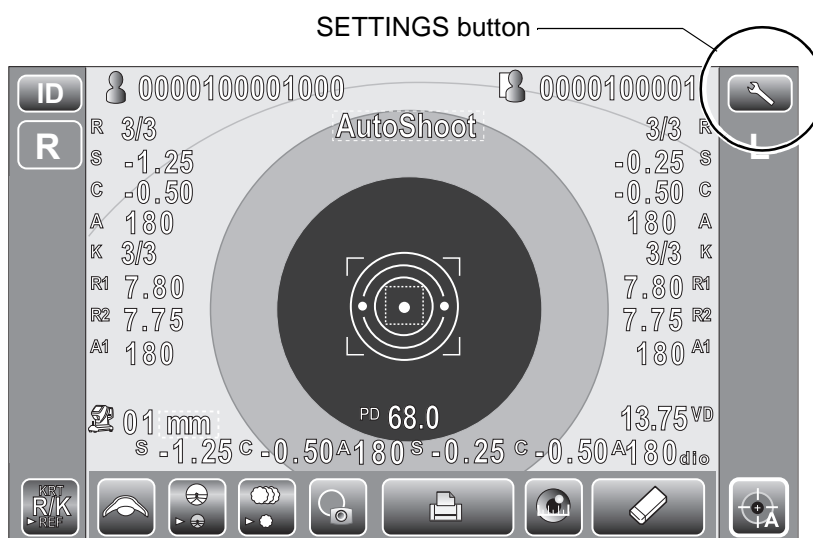


The SETUP screen is displayed.

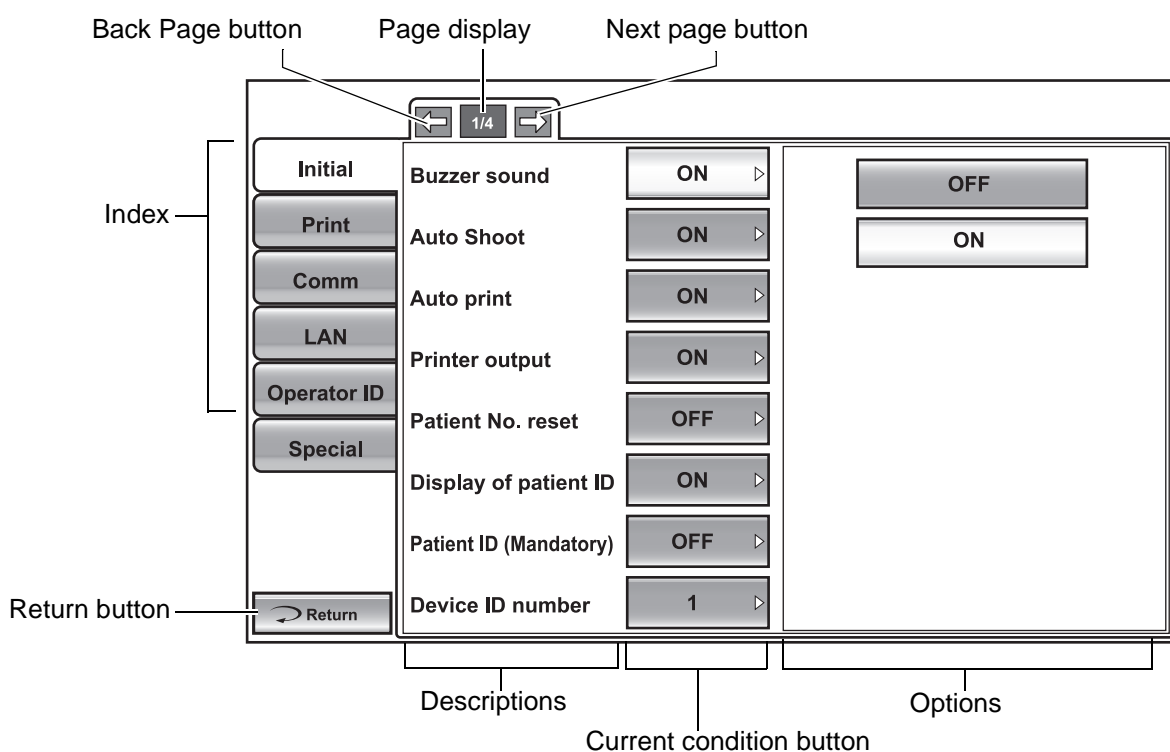


# OUTLINE OF SETUP SCREEN OPERATIONS


**1** Tap **INDEX** and select the subject of setting.

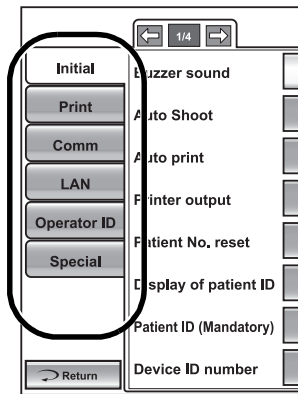


**2** Operate the **NEXT PAGE** button or **BACK PAGE** button, as necessary, and display the page to confirm/change.



**3** Tap the **CURRENT CONDITION** button of the item to be changed and find the **OPTIONS** button.

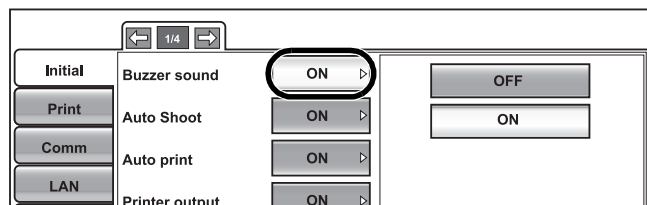


**4** Tap the **OPTIONS** button and change the setting.

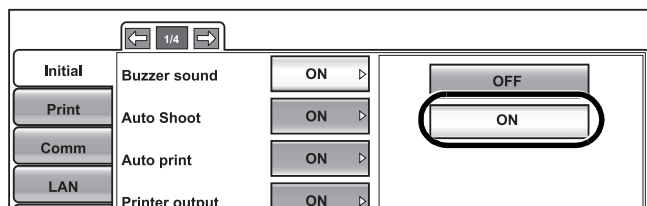

- Instead of the **OPTIONS** button, up/down buttons and ten-key would be displayed.


### TEN-KEY:

Tap ten-key on the screen and enter the figure. If there are several windows to enter, tap the window to enter the figure by ten-key. Tap **OK** and fix the input value.

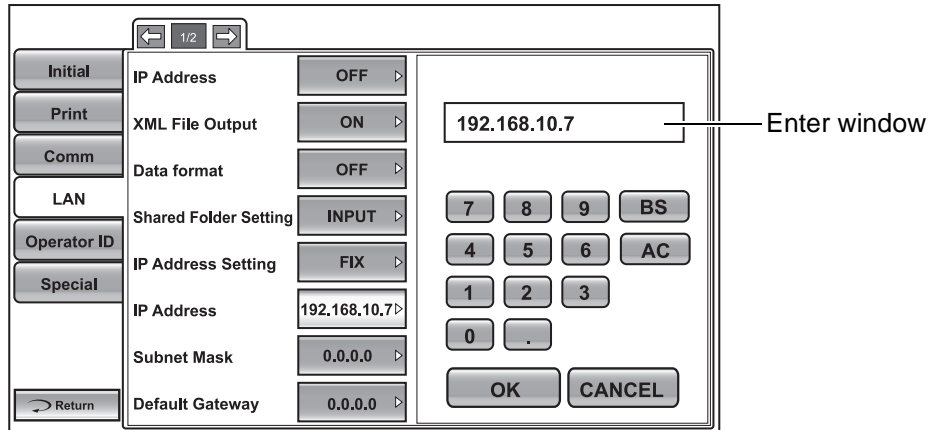


### KEYBOARD:

Tap keyboard on the screen and enter characters. If there are several windows to enter, tap the window to enter the figure by keyboard. Tap **OK** and fix the input value.

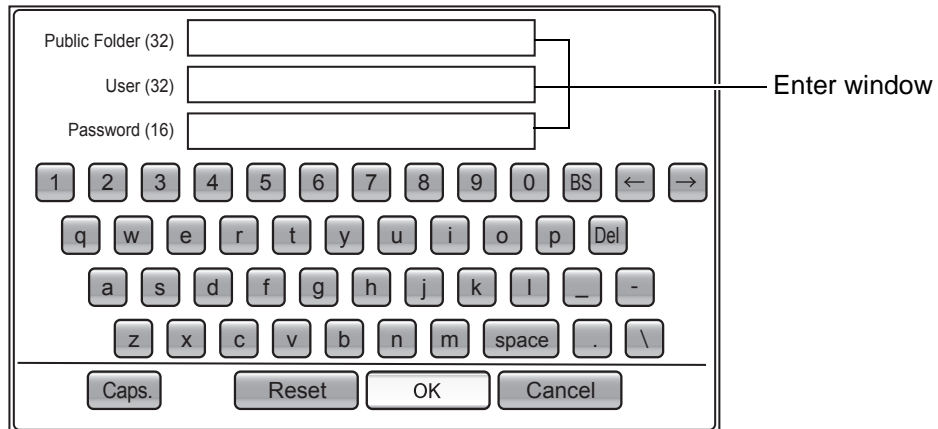


## RETURNING TO THE MEASUREMENT SCREEN

**1** Tap the **RETURN** button.

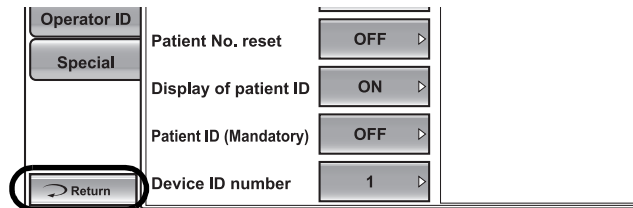

**2** The Measurement screen is displayed.

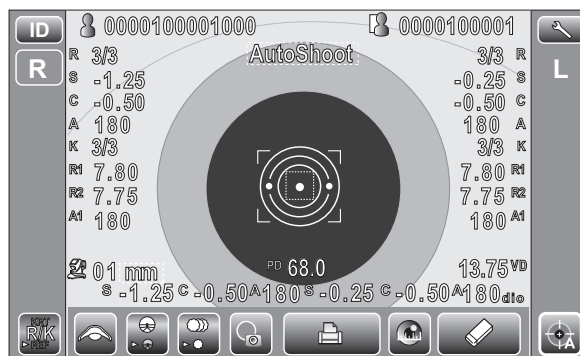

## LIST OF SETUP ITEMS

Setup items are categorized into 6 large indexes.

- "Initial" .....items related to the initial status after power on
- "Print" .....items related to output from the internal printer
- "Comm" .....items related to data output with the external device
- "LAN" .....items related to output using the LAN
- "Operator ID" .....items related to Operator ID
- "Special" .....items related to maintenance (for service engineer only)

### **INITIAL (INITIAL SETTING)**

Initial contains settings related to the initial status after power on, clearing all measurement values, etc.

Descriptions	Options	Details	Initial value
Buzzer sound	OFF	Buzzer does not sound.	ON
	ON	Buzzer sounds.	
Auto Shoot*	OFF	Default measurement mode is Manual.	ON
	ON	Default measurement mode is Auto Shoot.	
Auto print*	OFF	Not printed automatically.	ON
	ON	After AUTO measurement, results are printed out automatically.	
Printer output	OFF	Internal printer is disabled.	ON
	ON	Internal printer is active.	
Patient No. reset	OFF	Patient No. is not reset upon power on.	ON
	ON	Patient No. is reset upon power on.	
Display of patient ID	OFF	Patient ID is not displayed.	OFF
	ON	Patient ID is displayed.	
Patient ID (Mandatory)	OFF	Patient ID is not displayed.	OFF
	ON	Patient ID is displayed.	
Device ID number	1-99 Set by ten-key display.	Sets the Device ID number.	1
Display of Device ID num.	OFF	Device ID is not required.	OFF
	ON	Device ID is required.	
Start time of sleep mode	OFF	Power save function is not used.	10min
	1min	Power save status in 1min after last operation.	
	5min	Power save status in 5min after last operation.	
	10min	Power save status in 10min after last operation.	
	20min	Power save status in 20min after last operation.	
	30min	Power save status in 30min after last operation.	
60min	Power save status in 60min after last operation.		
Number of auto-shoot	1-10 Set by ten-key display.	The number of continuous measurements	3
Fog timing	Every time	Fog timing is applied every time.	Once
	Once	Fog timing is applied only once before the 1st measurement.	
Date/Time	Set by ten-key display.	Sets year, month, day, time (24hrs), minute and second	Installation date/time
Sph/Cyl step	0.12	Sph/Cyl is displayed by 0.12D step.	0.25
	0.25	Sph/Cyl is displayed by 0.25D step.	
Axis step	1°	Axial angle is displayed by 1° step	1°
	5°	Axial angle is displayed by 5° step	
VD	0.00	VD value is set to 0mm (contact lens).	13.75
	12.00	VD value is set to 12.00mm (eyeglass lens).	
	13.75	VD value is set to 13.75mm (eyeglass lens).	



Descriptions	Options	Details	Initial value
ADD	NO 40-44 45-49 50-54 55-59 60-64 65-69 70-74	The typical additional power for the age can be selected.	NO
D or mm(KRT)*	D	D (diopter) of corneal refractive power	mm
	mm	mm of corneal curvature	
HV or R1R2*	HV	Corneal curvature radius measurement result on screen is displayed by HV	R1R2
	R1R2	Corneal curvature radius measurement result on screen is displayed by R1R2(flat/steep meridian).	
Display of KRT unit*	OFF	KRT unit is not shown.	ON
	ON	KRT unit is shown.	
Cylinder sign	-	Cylinder sign is "-".	-
	+	Cylinder sign is "+".	
	MIX	Cylinder sign is "+" and "-".	
Measure mode setting*	REF	Default measurement mode is REF.	REF/KRT
	REF/KRT	Default measurement mode is R/K.	
	KRT	Default measurement mode is KRT.	
R/L or OD/OS	R/L	Right/left eyes is displayed by R/L.	R/L
	OD/OS	Right/left eyes is displayed by OD/OS.	
Control panel brightness	Level 1 (dark)	The brightness of control panel.	Level 4
	Level 2		
	Level 3		
	Level 4 (bright)		
Display of REF average	OFF	REF average is not displayed.	OFF
	ON	REF average is displayed.	
Shaded character	OFF	Font style of measurement values is not shaded.	ON
	ON	Font style of measurement values is shaded.	

\* : Only in KR-800

## SETTING OF INTERNAL PRINTER (PRINT)

Print contains settings related to output from the internal printer.

	Description	Options	Details	Initial value
Preset	-	All	Print format of preset is All. (For the details of "All," refer to "PRINTOUT FORMAT SETTING" on page 18.)	All
	-	Ave	Print format of preset is Ave. (For the details of "Ave," refer to "PRINTOUT FORMAT SETTING" on page 18.)	
	-	Classic*	Print format of preset is Classic. (For the details of "Classic," refer to "PRINTOUT FORMAT SETTING" on page 18.)	
Common	Barcode	OFF	Barcode is not printed.	OFF
		ON	Barcode is printed.	
	Operator ID	OFF	Operator ID is not printed.	OFF
		ON	Operator ID is printed.	
	Name	OFF	"Name" space is not available.	OFF
		ON	"Name" space is available.	
	Date	OFF	Date is not printed.	ON
		ON	Date is printed.	
	Date style	YMD	Print in Year/Month/Day format.	MDY
		MDY	Print in Month/Day/Year format.	
		DMY	Print in Day/Month/Year format.	
	Patient No./Patient ID	OFF	Patient No./Patient ID is not printed.	OFF
		ON	Patient No./Patient ID is printed.	
	Device ID	OFF	Device ID No. is not printed.	OFF
		ON	Device ID No. is printed.	
	Serial number	OFF	Serial No. is not printed.	ON
		ON	Serial No. is printed.	
	Include error data	OFF	"Error" data is not printed.	OFF
		ON	"Error" data is printed.	
	TOPCON logo	OFF	TOPCON logo is not printed.	ON
		ON	TOPCON logo is printed.	
	Message print	OFF	Message is not printed.	OFF
		ON	Message is printed.	
	Input message	Set by keyboard display.	String of up to 72 characters.	NONE
Graphic print	Normal Printer	Picture of refractive condition is not printed.	Normal Printer	
	Graphic Printer	Picture of refractive condition is printed.		
Line space	0-24 Set by ten key display.	Line space is set in dot units.	0	
Auto Cut	OFF	Auto cut is carried out.	ON	
	ON	Auto cut is not carried out.		

\* : Only in KR-800

	Description	Options	Details	Initial value
REF/KRT (Print setting on R/K mode) *	Print Layout	DATA	Measurement values are printed in terms of REF or KRT.	DATA
		R/L	Measurement values are printed in terms of Right or Left.	
	VD	OFF	VD value (Vertex distance) is not printed.	ON
		ON	VD value (Vertex distance) is printed.	
	Cylinder sign	OFF	Cylinder sign is not printed.	ON
		ON	Cylinder sign is printed.	
	Print form of REF result	ALL	All refractive measurements are printed.	ALL
		AVE	Only averaged is printed.	
	Reliability	OFF	Reliability number is not printed.	OFF
		ON	Reliability number is printed.	
	S.E.	OFF	S.E. is not printed.	ON
		ON	S.E. is printed.	
	PD	OFF	PD value is not printed.	ON
		ON	PD values is printed.	
	ADD	OFF	ADD value is not printed.	OFF
		ON	ADD value is printed.	
	KRT print layout	D/mm	KRT data is printed as follows, D (corneal refractive power)/mm (corneal curvature).	D/mm
		mm/D	KRT data is printed as follows, mm (corneal curvature)/D (corneal refractive power).	
	Print form of KRT result	ALL	All measurement values are printed.	ALL
		AVE	Only average value are printed.	
	KRT ave. -HV or R1R2	HV	Kerato average in print out is HV (horizontal/vertical).	R1R2
		R1R2	Kerato average in print out is R1R2 (flat/steep meridian).	
	KRT data -HV or R1R2	HV	KRT measurement result is printed in HV (horizontal/vertical).	R1R2
		R1R2	KRT measurement result is printed in R1R2 (flat/steep meridian).	
	KRT average	OFF	KRT average value is not printed.	ON
		ON	KRT average value is printed.	
	KRT cylinder	OFF	Kerato-cylinder value and axial angle are not printed.	ON
		ON	Kerato-cylinder value and axial angle are printed.	
Corneal diameter	OFF	Corneal diameter is not printed.	ON	
	ON	Corneal diameter is printed.		
REF (Print setting on REF mode)	VD	OFF	VD value (Vertex distance) is not printed.	ON
		ON	VD value (Vertex distance) is printed.	
	Cylinder sign	OFF	Cylinder sign is not printed.	ON
		ON	Cylinder sign is printed.	
	Print form of REF result	ALL	All refractive measurements are printed.	ALL
		AVE	Only typical value is printed.	
	Reliability	OFF	Reliability number is not printed.	OFF
		ON	Reliability number is printed.	
	S.E.	OFF	S.E. is not printed.	ON
		ON	S.E. is printed.	
	PD	OFF	PD value is not printed.	ON
		ON	PD values is printed.	
	ADD	OFF	ADD value is not printed.	OFF
		ON	ADD value is printed.	

\* : Only in KR-800

	Description	Options	Details	Initial value
KRT (Print setting on KRT mode) *	KRT print layout	D/mm	KRT data is printed as follows, D (corneal refractive power)/mm (corneal curvature).	D/mm
		mm/D	KRT data is printed as follows, mm (corneal curvature)/D (corneal refractive power).	
	Print form of KRT result	ALL	Printout all measurement values.	ALL
		AVE	Printout only average value.	
	KRT ave. -HV or R1R2	HV	Display average of KRT measurement results is set to HV (horizontal/vertical).	R1R2
		R1R2	Display average of KRT measurement results is set to R1R2 (flat/steep meridian).	
	KRT data -HV or R1R2	HV	KRT measurement result is printed in simple format.	R1R2
		R1R2	KRT measurement result is printed in full format.	
	KRT average	OFF	Do not print KRT average value.	ON
		ON	Print KRT average value.	
	KRT cylinder	OFF	Do not print kerato-cylinder value and axial angle.	ON
		ON	Print kerato-cylinder value and axial angle.	
	Corneal diameter	OFF	Do not print corneal diameter.	ON
		ON	Print corneal diameter.	

\* : Only in KR-800

## DATA COMMUNICATION (COMM)

Comm contains settings related to data output with the external device.

Description	Options	Details	Initial value
Output data format*	REF	Only REF data are output.	ALL
	KRT	Only KRT data are output.	
	ALL	All data are output.	
Communication Format	OLD	OLD TOPCON format	OLD
	NEW	NEW TOPCON format	
	STD1	TOPCON STD1 format	
	STD2	TOPCON STD2 format	
	STD4	TOPCON STD4 format	
	CM1	Custom specification	
	CM4	Custom specification	
Use of Output port	OFF	RS-232C port is disabled.	OFF
	ON	RS-232C port is enabled.	
Baudrate setting	2400	Baudrate value:2400	2400
	9600	Baudrate value:9600	

\* : Only in KR-800

## LAN CONNECTION (LAN)

LAN contains settings related to data output via LAN.

Description	Options	Details	Initial value
IP Address	OFF	LAN connection is off.	OFF
	ON	LAN connection is on.	
XML File Output	OFF	XML file is not output.	OFF
	ON	XML file is output.	
Data format	OFF	Data is not output.	OFF
	STD2	REF/KRT data are output in TOPCON STD2 format	
	STD4	REF/KRT data are output in TOPCON STD4 format	
Shared Folder Setting	Shared Folder (up to 32 characters) User Name (up to 32 characters) Password (up to 16 characters) Set by keyboard display	Path and permission to shared folder is set.	NONE
IP Address Setting	FIX	Assign IP address manually.	FIX
	AUTO	Assign IP address automatically.	
IP Address	0.0.0.0 Set by ten-key display.	IP address of PC to output data.	NONE
Subnet Mask	0.0.0.0 Set by ten-key display.	Subnet mask address of RM-800/KR-800.	NONE
Default Gateway	0.0.0.0 Set by ten-key display.	Default gateway address of RM-800/KR-800.	NONE
Primary DNS Server	0.0.0.0 Set by ten-key display.	Primary DNS Server number.	NONE
Secondary DNS Server	0.0.0.0 Set by ten-key display.	Secondary DNS Server number.	NONE

## OPERATOR ID

OPERATOR contains settings related to Operator ID.

Description	Options	Details	Initial value
Use of Operator ID	OFF	Operator ID will be displayed on the control panel and output.	OFF
	ON	Operator ID will not be displayed on the control panel and output.	
Prefix of Ope. ID	Set by ten-key display. (up to 3 characters)	Set the Prefix of Operator ID can be registered.	NONE
Operator ID (Mandatory)	OFF	Operator ID is not required.	OFF
	ON	Operator ID is required.	
Fixed Ope. ID setting	OFF	Operator ID is not fixed.	OFF
	ON	Operator ID is fixed.	
Fixed Ope. ID entry	Set by ten-key display. (up to 13 characters)	Input fixed operator ID	NONE

## SPECIAL


SPECIAL is the mode for service engineer only; it can not be accessed.

# MAINTENANCE

## DAILY CHECKUPS

### CHECKING THE MEASURING ACCURACY

- The attached model eye should be measured and the accuracy checked at regular intervals.
- To set up the model eye, insert the guide groove of the model eye to the chinrest tissue pin.
- Set the display step of spherical/cylindrical to 0.12D and perform measurement.

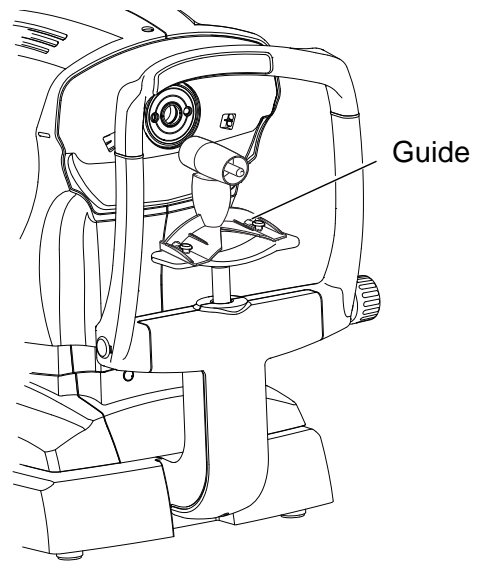

If the measurement result is widely different from the value shown on the model eye, call your dealer or TOPCON at the address on back cover.

### CLEANING THE INSTRUMENT

- Dust on measuring window... Blow off dust with a blower.
- Fingerprints and oil spots on measuring window  
..... Blow off dust by a blower and wipe the surface gently with a camera lens cleaner using clean gauze.
- Dirty instrument cover..... Wipe the surface with the attached silicon cloth or a dry soft cloth. Never use solvents or a chemical duster.

### CLEANING THE FOREHEAD REST AND CHIN REST

- Wipe the forehead rest and the chin rest with a cloth moistened with a tepid solution of neutral detergent for kitchenware.

## DAILY MAINTENANCE


- For this instrument, dust may cause errors. When not in use, replace the measuring lens cap and dust cover.
- When not in use, turn off the POWER switch.

## ORDERING CONSUMABLE ITEMS

- When ordering consumable items, tell the product name, product code and quantity to your dealer or TOPCON at the address of back cover.

Product name	Product code
Chinrest tissue	40310 4082
Silicon cloth	44800 1001
Dust cover	42360 9002

Product name	Product code
Printer paper	44800 4001

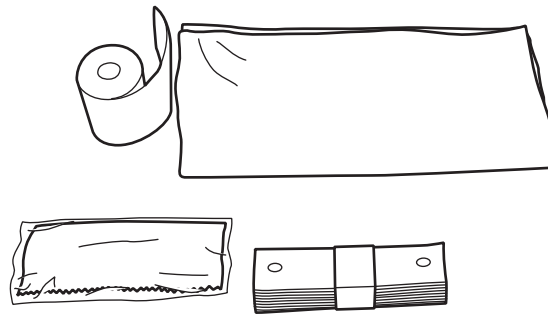



## USER MAINTENANCE ITEM

Item	Inspection time	Contents
Inspection	Before using	The instrument works properly. The objective lens must be free of stain or flaw.
Cleaning	When the part is stained	Objective lens External cover, control panel, etc.


## BRIGHTNESS ADJUSTMENT OF CONTROL PANEL


- The control panel is optimally adjusted when shipped.
- For control panel brightness adjustment, see "INITIAL (INITIAL SETTING)," "Control panel brightness" (page 47).

## PRINTER PAPER JAM

 <b>CAUTION</b>	<ul style="list-style-type: none"><li>• To avoid failure or potential injury, do not open the printer cover while the printer is in operation.</li><li>• To avoid potential injury in case of malfunction, including a paper jam, be sure to shut off the power before attempting to repair it.</li><li>• To avoid potential injury, do not touch the printer body including metal parts or the paper cutter, while the printer is in operation or when replacing the printer paper.</li><li>• Pay much attention not to touch the internal printer's body when the cover is open. If touched, it may result in trouble due to electrostatic discharge.</li></ul>
 <b>NOTE</b>	If the printer paper is jammed in the printer, printing will stop and the jam should be cleared.

- 1** Open the printer cover, and take out the jammed paper pieces.





 <b>NOTE</b>	After removing the jammed printer paper, tap the Print button to print out the previous measurement data. If no previous measurement data has saved, a blank sheet is printed out.
---	---




## SUPPLYING THE CHINREST TISSUE

- When the chinrest tissue has run out, pull off chinrest tissue pins and place new tissue.

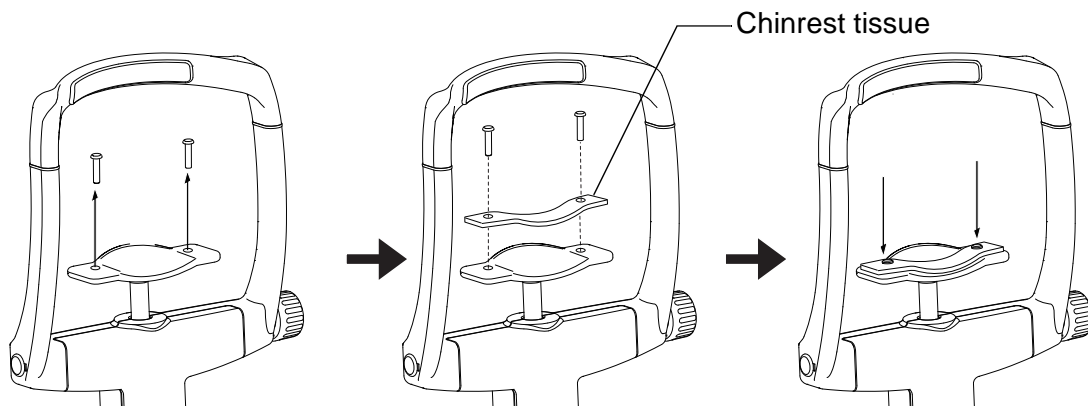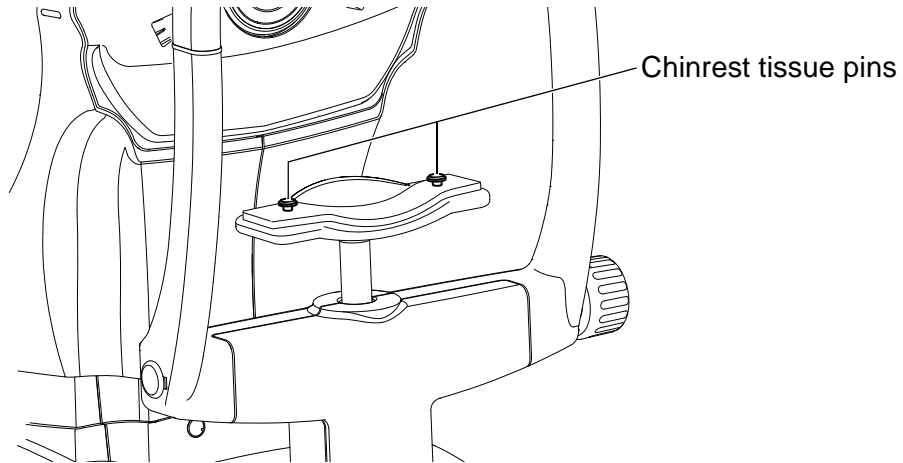


## **MAINTENANCE**

### **CLEANING THE KERATO RING AND THE COVER**

 <b>NOTE</b>	Do not clean plastic parts with solvents. Benzine, thinner, ether and gasoline may cause discoloring and decomposition.
---	---

- 1** If the kerato ring and the cover get soiled, wipe the surface with dry cloth.
- 2** If the kerato ring and the cover are noticeably stained, wipe the surface with a damp cloth which is moistened in a tepid water solution of neutral detergent.

### **CLEANING THE CONTROL PANEL**

 <b>NOTE</b>	<ul style="list-style-type: none"><li>• As the control panel screen is a touch panel, be sure to turn off the POWER switch before wiping. The touch panel will react and malfunction.</li><li>• When the monitor cleaner has become dirty, wash it. When washing, rinse it thoroughly so no detergent is left. If the detergent is left, it may cause uneven wiping.</li></ul>
---	--

#### **CONTAMINATION BY DUST**

Remove the dust with a soft brush, and wipe with the attached monitor cleaner.

#### **CONTAMINATION BY FINGERPRINTS**

Wipe with the attached monitor cleaner.

If the stain still remains, moisten the monitor cleaner with water and then wipe off the stain.

# TROUBLESHOOTING

## TROUBLE-SHOOTING OPERATIONS

### MESSAGE LIST

"OVER-SPH"	Spherical power exceeds +22D or -25D.
"OVER-CYL"	Cylindrical power exceeds $\pm 10D$ .
"OVER-R" *	Corneal curvature exceeds 5.00-10.00mm.
"NO TARGET"	There is no target or the eye image is too dark.
"AGAIN"	There is more than $\pm 5D$ difference from the previous measurement value.
"NO CENTER"	Center of eye can not be found.
"ERROR"	The patient's eye blinks or moves during measurement. If this message appears while with measuring model eye, the instrument may have a problems. Contact your service engineer.
"ALIGN ERR" *	The alignment is significantly failed during the measurement.
"LAN hostname Error"	Failed in host name resolution of the destination (to be connected with the share folder). Confirm the inputted host name or DNS server address.
"LAN mount Error"	Failed in connection with the share folder. Confirm the address, folder name, user name and password of the destination (to be connected with the share folder).
"LAN create Error"	Failed in file creation. Confirm that write permission to the share folder is set correctly.
"LAN write Error"	Failed in writing to the file. Check the free space capacity at the save location.
"RS-232C FAIL"	Failed in RS-232C data transmission.
"Please check the DATE/TIME"	The battery for the built-in clock become run down. Before using, confirm the time and date on the SETUP menu. If the message comes up frequently, call your service engineer.
"Previous measurements are left. Please press the Clear button."	Displayed when the output of all output-set data fails.

\* : Only in KR-800

## TROUBLE-SHOOTING OPERATIONS



### WARNING

To avoid electrical shock, do not open the instrument.  
All service should be performed by a qualified service engineer.

If a problem is suspected, use the following check list.

If following instructions does not improve the condition, or if your problem is not included in the list, contact your dealer or TOPCON at the address on the back cover.

### CHECK LIST

Trouble	Condition	Check	Page
Control panel does not turn on.	_____	Is power cable unplugged?	20
		Is power cable connected to the instrument?	20
Control panel is not clear.	The image is dark.	Adjust the brightness by "Control panel Brightness Adjust".	47
Any trouble is found in a movable part.	_____	Do not move it forcibly but call our service engineer.	27
Printing is not done.	Paper comes out without printing.	Confirm the direction of paper winding. If the direction is incorrect, reset paper to the proper direction.	22
	Paper does not come out.	If "PAPER END" displayed on control panel, replenish printer paper.	22

# SPECIFICATIONS AND PERFORMANCE

## SPECIFICATIONS AND PERFORMANCE

### RM-800

Range of Refractometry Measurement	Spherical refractive power: -25 to +22D (0.12D/0.25D steps) Cylindrical refractive power: 0D to $\pm 10$ D (0.12D/0.25D steps) Direction of astigmatic axis: 0° to 180° (1°/5° steps) (where, spherical refractive power + cylindrical refractive power $\leq +22$ D, or spherical refractive power + cylindrical refractive power $\leq -25$ D) Measured minimum pupil diameter: $\phi 2$ mm
PD measurement	20-85mm (0.5mm display unit)
External I/O terminal	USB(for Import), RS-232C(for Export), LAN(for Export)



#### **NOTE**

##### Essential performance

- Measurement must be performed correctly.
- Monitor screen display must not be distorted.



# GENERAL INFORMATION ON USAGE AND MAINTENANCE

## **INTENDED PATIENT POPULATION**

The patient who undergoes an examination by this instrument must maintain concentration for a few minutes and keep to the following instructions:

- To fix the face to the chinrest, forehead rest.
- To keep the eye open.
- To understand and follow instructions when undergoing an examination.

## **INTENDED USER PROFILE**

Since the Auto Refractometer RM-800, Auto Kerato-Refractometer KR-800 are medical devices, the operation should be supervised by a physician.

## **ENVIRONMENTAL CONDITIONS OF USE**

Temperature: 10°C to 40°C  
Humidity: 30% to 90% RH(without condensation)  
Atmospheric pressure: 700hPa to 1060hPa

## **STORAGE, USAGE PERIOD**

### 1. Environmental conditions (without package)

\*Temperature : 10°C to 40°C  
Humidity : 10% to 95% (without condensation)  
Air pressure : 700hPa to 1060hPa

\* THIS INSTRUMENT DOES NOT MEET THE TEMPERATURE REQUIREMENTS OF ISO 15004-1 FOR STORAGE. DO NOT STORE THIS INSTRUMENT IN CONDITIONS WHERE THE TEMPERATURE MAY RISE ABOVE 40°C OR FALL BELOW 10°C.

### 2. When storing the instrument, ensure that the following conditions are met:

- (1) The instrument must not be splashed with water.
- (2) Store the instrument away from environments where air pressure, temperature, humidity, ventilation, sunlight, dust, salty/sulfurous air, etc. could cause damage.
- (3) Do not store or transport the instrument on a slanted or uneven surface or in an area where it is subject to vibrations or instability.
- (4) Do not store the instrument where chemicals are stored or gas is generated.

### 3. Normal life span of the instrument:

8 years from delivery providing regular maintenance is performed [TOPCON data]

## **ENVIRONMENTAL CONDITIONS FOR PACKAGING IN STORAGE**

(Product in its normal transport and storage container as provided by manufacturer)

Temperature : -20°C to 50°C  
Humidity : 10% to 95%

## **ENVIRONMENTAL CONDITIONS FOR PACKAGING IN TRANSPORTATION**

(Product in its normal transport and storage container as provided by manufacturer)

Temperature : -40°C to 70°C

Humidity : 10% to 95%

## **ELECTRIC RATING**

Source voltage: 100-240V AC, 50-60Hz

Power input: 30-75VA

## **SAFETY DESIGNATIONS PER IEC 60601-1 STANDARD**

- Type of protection against electric shocks: Class I  
The Class I equipment provides means to connect itself to the protective grounding system of utilities to thereby independently provide protection against electric shocks by keeping connectable metal components nonconductive in case of a failure in the basic insulation.
- Degree of protection against electric shocks: B type applied component  
The B type applied component provides the specified degree of protection against electric shocks with regard to the reliability particularly of leak current, patient measuring current and protective utility connection (in case of Class I equipment).
- Degree of protection against harmful intrusion of water (IEC 60529): IPX0  
This product does not provide protection against intrusion of water.  
(The degree of protection against harmful ingress of water defined in IEC 60529 is IPX0)
- Classification by sterilization/disinfection method specified by manufacturer  
This product does not have a component requiring sterilization/disinfection.
- Classification by safety of use in air/flammable anesthetic gas, oxygen or nitrous oxide/flammable anesthetic gas atmosphere
  - Equipment not suited for use in air/flammable anesthetic gas, oxygen or nitrous oxide/flammable anesthetic gas atmosphere
  - This product should be used in an environment free of flammable anesthetic gas and other flammable gases.
- Classification by operation mode  
Continuous operation refers to an operation under normal load conditions, within the specified temperature and without limitations on the operating time.

## **DIMENSIONS AND WEIGHT**

Dimensions: 317~341mm(W) × 521~538mm(D) × 447~477mm(H)

Weight : 15kg



## OPERATION PRINCIPLE

### Refraction (REF)


The instrument projects a near infra red ring of light onto the retina and the reflection of the ring is captured by a CCD camera. An internal computer analyzes the image and calculates the spherical, cylindrical and axial values.

### Keratometry (KRT)

The instrument projects a near infra red ring of light onto the cornea and the reflection of the ring is captured by a CCD camera. An internal computer analyzes the image and calculates the curvature radius, corneal astigmatic axis and the corneal refractive values.

## DISPOSAL

When disposing of the instrument and/or parts, follow local regulations for disposal and recycling.

 <b>NOTE</b>	<p><b>[WARNING]</b> Handling the cord on this product or cords associated with accessories sold with this product, will expose you to lead, a chemical known to the State of California to cause birth defects or other reproductive harm. <b>Wash hands after handling.</b></p> <p>This product contains a CRL Lithium Battery which contains Perchlorate Material-special handling may apply. See <a href="http://www.dtsc.ca.gov/hazardouswaste/perchlorate/">http://www.dtsc.ca.gov/hazardouswaste/perchlorate/</a> Note; This is applicable to California, U.S.A. only</p>
---	---

## **ELECTROMAGNETIC COMPATIBILITY**

The product conforms to the EMC standard (IEC 60601-1-2 Ed3.0:2007)

- a) MEDICAL ELECTRICAL EQUIPMENT needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the ACCOMPANYING DOCUMENTS.
- b) Portable and mobile RF communications equipment can affect MEDICAL ELECTRICAL EQUIPMENT.
- c) The use of ACCESSORIES, transducers and cables other than those specified, with the exception of transducers and cables sold by the manufacturer of the EQUIPMENT or SYSTEM as replacement parts for internal components, may result in increased EMISSIONS or decreased IMMUNITY of the EQUIPMENT or SYSTEM.
- d) The EQUIPMENT or SYSTEM should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the EQUIPMENT or SYSTEM should be observed to verify normal operation in the configuration in which it will be used.
- e) The use of the ACCESSORY, transducer or cable with EQUIPMENT and SYSTEMS other than those specified may result in increased EMISSION or decreased IMMUNITY of the EQUIPMENT or SYSTEM.

<b>Guidance and manufacturer's declaration - electromagnetic emissions</b>		
The RM-800/KR-800 is intended for use in the electromagnetic environment specified below. The customer or the user of the RM-800/KR-800 should assure that it is used in such an environment.		
<b>Emissions test</b>	<b>Compliance</b>	<b>Electromagnetic environment - guidance</b>
RF emissions CISPR 11	Group 1	The RM-800/KR-800 uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The RM-800/KR-800 is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC61000-3-2	Complies	
Voltage fluctuations/ flicker emissions IEC61000-3-3	Complies	

**Guidance and manufacturer's declaration - electromagnetic immunity**


The RM-800/KR-800 is intended for use in the electromagnetic environment specified below.  
The customer or the user of the RM-800/KR-800 should assure that it is used in such an environment.

<b>Immunity test</b>	<b>IEC 60601 test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment - guidance</b>
Electrostatic discharge(ESD) IEC 61000-4-2	± 6 kV contact  ± 8 kV air	± 6 kV contact  ± 8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply lines  ± 1 kV for input/output lines	± 2 kV for power supply lines  ± 1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 1 kV line(s) to line(s)  ± 2 kV line(s) to earth	± 1 kV line(s) to line(s)  ± 2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and Voltage variations on power supply input lines IEC 61000-4-11	<5% $U_t$ (>95% dip in $U_t$ ) for 0, 5 cycle 40% $U_t$ (60% dip in $U_t$ ) for 5 cycles 70% $U_t$ (30% dip in $U_t$ ) for 25 cycles <5% $U_t$ (>95% dip in $U_t$ ) for 5 sec.	<5% $U_t$ (>95% dip in $U_t$ ) for 0, 5 cycle 40% $U_t$ (60% dip in $U_t$ ) for 5 cycles 70% $U_t$ (30% dip in $U_t$ ) for 25 cycles <5% $U_t$ (>95% dip in $U_t$ ) for 5 sec.	Mains power quality should be that of a typical commercial or hospital environment. If the user or the RM-800/KR-800 requires continued operation during power mains interruptions, it is recommended that the RM-800/KR-800 be powered from an uninterruptible power supply or battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

NOTE  $U_t$  is the a.c. mains voltage prior to application of the test level.

**Guidance and manufacturer's declaration - electromagnetic immunity**

The RM-800/KR-800 is intended for use in the electromagnetic environment specified below.  
The customer or the user of the RM-800/KR-800 should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
<p>Conducted RF IEC 61000-4-6</p> <p>Radiated RF IEC 61000-4-3</p>	<p>3 Vrms 150kHz to 80MHz</p> <p>3 V/m 80MHz to 2, 5GHz</p>	<p>3 V</p> <p>3 V/m</p>	<p>Portable and mobile RF communications equipment should be used no closer to any part of the RM-800/KR-800, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance</p> $d = 1.2 \sqrt{P}$ $d = 1.2 \sqrt{P} \quad 80\text{MHz to } 800\text{MHz}$ $d = 2.3 \sqrt{P} \quad 800\text{MHz to } 2, 5\text{GHz}$ <p>where <math>P</math> is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and <math>d</math> is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,<sup>a</sup> should be less than the compliance level in each frequency range.<sup>b</sup></p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 

NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

<sup>a</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the RM-800/KR-800 is used exceeds the applicable RF compliance level above, the RM-800/KR-800 should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the RM-800/KR-800.

<sup>b</sup> Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

**Recommended separation distance between  
portable and mobile RF communications equipment and the RM-800/KR-800**

The RM-800/KR-800 is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the RM-800/KR-800 can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the RM-800/KR-800 as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150kHz to 80MHz $d = 1.2 \sqrt{P}$	80MHz to 800MHz $d = 1.2 \sqrt{P}$	800MHz to 2,5GHz $d = 2.3 \sqrt{P}$
0, 01	0, 12	0, 12	0, 23
0, 1	0, 38	0, 38	0, 73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.  
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

**REQUIREMENTS FOR THE EXTERNAL DEVICE**

The external device connected to the analog and digital interfaces must comply with the respective IEC or ISO standards (e.g. IEC 60950-1 for data processing equipment and IEC 60601-1 for medical equipment).


Anybody connecting additional equipment to medical electrical equipment configures a medical system and is therefore responsible that the system complies with the requirements for medical electrical systems. Attention is drawn to the fact that local laws take priority over the above mentioned requirements. If in doubt, contact your dealer or TOPCON (see the back cover).

## **PATIENT'S ENVIRONMENT**

When the patient or inspector may touch the devices (including the connecting devices) or when the patient or inspector may touch the person that comes into contact with the devices (including the connecting devices), the patient's environment is shown below.

In the patient's environment, use the device conforming to IEC60601-1. If you are compelled to use any device not conforming to IEC60601-1, use an insulation transformer or the common protective earth system.

Do not use the power strip in the patient's environment. Connect the power supply of the device to the commercial power supply.

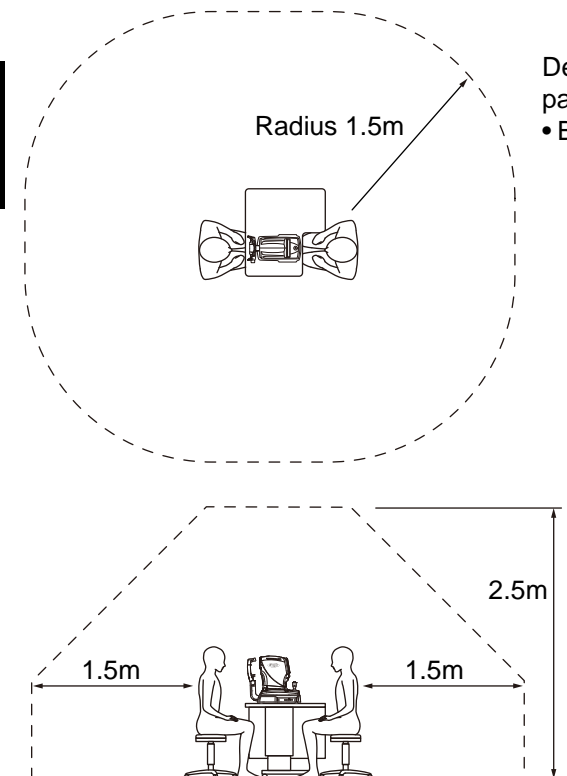

Devices applicable to the patient's environment  
• Barcode reader (Note 1)

Note 1: Use the device conforming to IEC60950-1.



### **CAUTION**

- Don't connect an additional power strip or an extension cord to the system.
- Don't connect the device which is not recognized as one component of the system.

# REFERENCE

## OPTIONAL ACCESSORIES


- Adjustable instrument table AIT-16

The table height can be adjusted to facilitate measurement.

### Specifications

- Dimensions.....525(W)x490(D)mm
- Table height.....660~880mm
- Table size .....490x500mm
- Weight .....approx. 23kg
- Power consumption..... 150VA (100-120V, 220-240V)

- RS-232C on-line cable

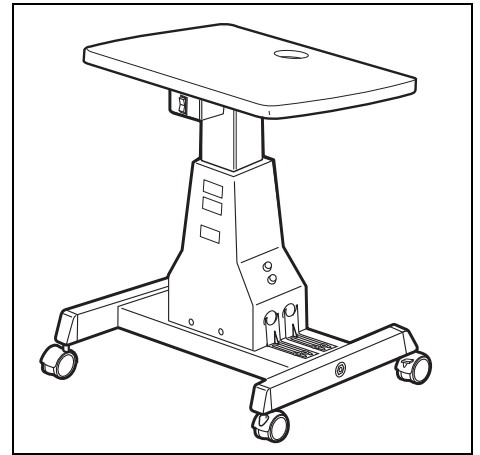

## SHAPE OF PLUG

Country	Voltage/frequency	Shape of plug
Mexico	110V/50Hz	Type C&E
Argentina	220V/60Hz	Type A
Peru	220V/60Hz	Type A
Venezuela	110V/50Hz	Type C&E
Bolivia & Paraguay	220V/60Hz	Type A (Most common) Type H (Infrequently)
Chile	220V/60Hz	Type A
Colombia	110V/50Hz	Type C
Brazil	220V/60Hz 127V/60Hz	Type A Type C
Ecuador	110V/50Hz	Type C&E
USA	120V/60Hz	Type A (Hospital Grade)
Canada	120V/60Hz	Type A (Hospital Grade)

# IPA FONT LICENSE AGREEMENT v1.0

The Licensor provides the Licensed Program (as defined in Article 1 below) under the terms of this license agreement ("Agreement"). Any use, reproduction or distribution of the Licensed Program, or any exercise of rights under this Agreement by a Recipient (as defined in Article 1 below) constitutes the Recipient's acceptance of this Agreement.

## Article 1 (Definitions)

1. "Digital Font Program" shall mean a computer program containing, or used to render or display fonts.
2. "Licensed Program" shall mean a Digital Font Program licensed by the Licensor under this Agreement.
3. "Derived Program" shall mean a Digital Font Program created as a result of a modification, addition, deletion, replacement or any other adaptation to or of a part or all of the Licensed Program, and includes a case where a Digital Font Program newly created by retrieving font information from a part or all of the Licensed Program or Embedded Fonts from a Digital Document File with or without modification of the retrieved font information.
4. "Digital Content" shall mean products provided to end users in the form of digital data, including video content, motion and/or still pictures, TV programs or other broadcasting content and products consisting of character text, pictures, photographic images, graphic symbols and/or the like.
5. "Digital Document File" shall mean a PDF file or other Digital Content created by various software programs in which a part or all of the Licensed Program becomes embedded or contained in the file for the display of the font ("Embedded Fonts"). Embedded Fonts are used only in the display of characters in the particular Digital Document File within which they are embedded, and shall be distinguished from those in any Digital Font Program, which may be used for display of characters outside that particular Digital Document File.
6. "Computer" shall include a server in this Agreement.
7. "Reproduction and Other Exploitation" shall mean reproduction, transfer, distribution, lease, public transmission, presentation, exhibition, adaptation and any other exploitation.
8. "Recipient" shall mean anyone who receives the Licensed Program under this Agreement, including one that receives the Licensed Program from a Recipient.

## Article 2 (Grant of License)

The Licensor grants to the Recipient a license to use the Licensed Program in any and all countries in accordance with each of the provisions set forth in this Agreement. However, any and all rights underlying in the Licensed Program shall be held by the Licensor. In no sense is this Agreement intended to transfer any right relating to the Licensed Program held by the Licensor except as specifically set forth herein or any right relating to any trademark, trade name, or service mark to the Recipient.

1. The Recipient may install the Licensed Program on any number of Computers and use the same in accordance with the provisions set forth in this Agreement.
2. The Recipient may use the Licensed Program, with or without modification in printed materials or in Digital Content as an expression of character texts or the like.
3. The Recipient may conduct Reproduction and Other Exploitation of the printed materials and Digital Content created in accordance with the preceding Paragraph, for commercial or non-commercial purposes and in any form of media including but not limited to broadcasting, communication and various recording media.
4. If any Recipient extracts Embedded Fonts from a Digital Document File to create a Derived Program, such Derived Program shall be subject to the terms of this agreement.
5. If any Recipient performs Reproduction or Other Exploitation of a Digital Document File in which Embedded Fonts of the Licensed Program are used only for rendering the Digital Content within such Digital Document File then such Recipient shall have no further obligations under this Agreement in relation to such actions.
6. The Recipient may reproduce the Licensed Program as is without modification and transfer such copies, publicly transmit or otherwise redistribute the Licensed Program to a third party for commercial or non-commercial purposes ("Redistribute"), in accordance with the provisions set forth in Article 3 Paragraph 2.
7. The Recipient may create, use, reproduce and/or Redistribute a Derived Program under the terms stated above for the Licensed Program: provided, that the Recipient shall follow the provisions set forth in Article 3 Paragraph 1 when Redistributing the Derived Program.

## Article 3 (Restriction)

The license granted in the preceding Article shall be subject to the following restrictions:

1. If a Derived Program is Redistributed pursuant to Paragraph 4 and 7 of the preceding Article, the following conditions must be met:
  - (1)The following must be also Redistributed together with the Derived Program, or be made available online or by means of mailing mechanisms in exchange for a cost which does not exceed the total costs of postage, storage medium and handling fees:
    - (a) a copy of the Derived Program; and
    - (b) any additional file created by the font developing program in the course of creating the Derived Program that can be used for further modification of the Derived Program, if any.
  - (2)It is required to also Redistribute means to enable recipients of the Derived Program to replace the Derived Program with the Licensed Program first released under this License (the "Original Program"). Such means may be to provide a difference file from the Original Program, or instructions setting out a method to replace the Derived Program with the Original Program.
  - (3)The Recipient must license the Derived Program under the terms and conditions of this Agreement.
  - (4)No one may use or include the name of the Licensed Program as a program name, font name or file name of the Derived Program.
  - (5) Any material to be made available online or by means of mailing a medium to satisfy the requirements of this paragraph may be provided, verbatim, by any party wishing to do so.
2. If the Recipient Redistributes the Licensed Program pursuant to Paragraph 6 of the preceding Article, the Recipient shall meet all of the following conditions:
  - (1)The Recipient may not change the name of the Licensed Program.
  - (2)The Recipient may not alter or otherwise modify the Licensed Program.
  - (3)The Recipient must attach a copy of this Agreement to the Licensed Program.
3. THIS LICENSED PROGRAM IS PROVIDED BY THE LICENSOR "AS IS" AND ANY EXPRESSED OR IMPLIED WARRANTY AS TO THE LICENSED PROGRAM OR ANY DERIVED PROGRAM, INCLUDING, BUT NOT LIMITED TO, WARRANTIES OF TITLE, NON-INFRINGEMENT, MERCHANTABILITY, OR FITNESS FOR A PARTICULAR PURPOSE, ARE DISCLAIMED. IN NO EVENT SHALL THE LICENSOR BE LIABLE FOR ANY DIRECT, INDIRECT, INCIDENTAL, SPECIAL, EXTENDED, EXEMPLARY, OR CONSEQUENTIAL DAMAGES (INCLUDING, BUT NOT LIMITED TO; PROCUREMENT OF SUBSTITUTED GOODS OR SERVICE; DAMAGES ARISING FROM SYSTEM FAILURE; LOSS OR CORRUPTION OF EXISTING DATA OR PROGRAM; LOST PROFITS), HOWEVER CAUSED AND ON ANY THEORY OF LIABILITY, WHETHER IN CONTRACT, STRICT LIABILITY OR TORT (INCLUDING NEGLIGENCE OR OTHERWISE) ARISING IN ANY WAY OUT OF THE INSTALLATION, USE, THE REPRODUCTION OR OTHER EXPLOITATION OF THE LICENSED PROGRAM OR ANY DERIVED PROGRAM OR THE EXERCISE OF ANY RIGHTS GRANTED HEREUNDER, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.
4. The Licensor is under no obligation to respond to any technical questions or inquiries, or provide any other user support in connection with the installation, use or the Reproduction and Other Exploitation of the Licensed Program or Derived Programs thereof.

## Article 4 (Termination of Agreement)

1. The term of this Agreement shall begin from the time of receipt of the Licensed Program by the Recipient and shall continue as long as the Recipient retains any such Licensed Program in any way.
2. Notwithstanding the provision set forth in the preceding Paragraph, in the event of the breach of any of the provisions set forth in this Agreement by the Recipient, this Agreement shall automatically terminate without any notice. In the case of such termination, the Recipient may not use or conduct Reproduction and Other Exploitation of the Licensed Program or a Derived Program: provided that such termination shall not affect any rights of any other Recipient receiving the Licensed Program or the Derived Program from such Recipient who breached this Agreement.

## Article 5 (Governing Law)

1. IPA may publish revised and/or new versions of this License. In such an event, the Recipient may select either this Agreement or any subsequent version of the Agreement in using, conducting the Reproduction and Other Exploitation of, or Redistributing the Licensed Program or a Derived Program. Other matters not specified above shall be subject to the Copyright Law of Japan and other related laws and regulations of Japan.
2. This Agreement shall be construed under the laws of Japan.



---

Please specify the following when contacting us regarding questions about this operation microscope.

- Model name: RM-800,KR-800
- Serial No.: Marked on the rating nameplate.
- Period of use: Please inform us of the date of purchase.
- Defective condition: Please provide us with as much detail as possible.

---

AUTO REFRACTOMETER RM-800  
AUTO KERATO-REFRACTOMETER KR-800

USER MANUAL

2012 version (2012.10-50LW0)

Date of issue: October 1, 2012

Published by TOPCON CORPORATION

75-1 Hasunuma-cho, Itabashi-ku, Tokyo, 174-8580 Japan.

## AUTO REFRACTOMETER

# RM-800

## AUTO KERATO-REFRACTOMETER

# KR-800

---

### TOPCON MEDICAL SYSTEMS, INC.

111 Bauer Drive, Oakland, NJ 07436, USA Phone:+1-201-599-5100 Fax:+1-201-599-5250 www.topconmedical.com

### TOPCON CANADA INC.

110 Provencher Avenue, Boisbriand, QC J7G 1N1 CANADA Phone:+1-450-430-7771 Fax:+1-450-430-6457 www.topcon.ca

### TOPCON EUROPE MEDICAL B.V.

(European Representative)(European Sole Sales Company)

Essebaan 11; 2908 LJ Capelle a/d IJssel; P.O.Box145; 2900 AC Capelle a/d IJssel; THE NETHERLANDS  
Phone:+31-(0)10-4585077 Fax:+31-(0)10-4585045 E-mail: medical@topcon.nl; www.topcon.eu

#### ITALY OFFICE

:Viale dell'Industria 60; 20037 Paderno Dugnano; (Milano), ITALY Phone:+39-02-9186671 Fax:+39-02-91081091 E-mail: topconitaly@tiscali.it; www.topcon.it

#### DANMARK OFFICE

:Praestemarksvej 25; 4000 Roskilde, DANMARK Phone:+45-46-327500 Fax:+45-46-327555 E-mail: topcon@topcondanmark.dk www.topcondanmark.dk

#### IRELAND OFFICE

:Unit 276, Blanchardstown; Corporate Park 2 Ballycoolin Dublin 15, IRELAND Phone:+353-18975900 Fax:+353-18293915 E-mail: medical@topcon.ie; www.topcon.ie

### TOPCON DEUTSCHLAND G.m.b.H.

Hanns-Martin-Schleyer Strasse 41; D-47877 Willich, GERMANY Phone:+49-(0)2154-8850 Fax:+49-(0)2154-885177 E-mail:med@topcon.de; www.topcon.de

### TOPCON ESPAÑA S.A.

HEAD OFFICE:Frederic Mompou 4 Esc. A Bajos 3, 08960 Sant Just Desvern Barcelona, Spain Phone:+34-93-4734057 Fax:+34-93-4733932 E-mail: medica@topcon.es; www.topcon.es  
PORTUGAL OFFICE:Rua da Forte,6-6A,L-0.22,2790-072 Camaxide, PORTUGAL Phone:+351-210-994626 Fax:+351-210-938786 www.topcon.pt

### TOPCON S.A.R.L.

BAT A1 3 route de la révolte 93206 SAINT DENIS CEDEX, FRANCE Phone:+33 1 49 21 23 23 Fax:+33 1 49 21 23 24 E-mail:topcon@topcon.fr; www.topcon.fr

### TOPCON SCANDINAVIA A.B.

Neogatan 2; P.O.Box 25; 43151 Mölndal, SWEDEN Phone:+46-(0)31-7109200 Fax:+46-(0)31-7109249 E-mail:medical@topcon.se; www.topcon.se

### TOPCON ( GREAT BRITAIN ) LTD.

Topcon House,Kennet Side,Bone Lane,Newbury,Berkshire RG14 5PX United Kingdom  
Phone:+44-(0)1635-551120 Fax:+44-(0)1635-551170 E-mail: info@topcon.co.uk; www.topcon.co.uk

### TOPCON POLSKA Sp. z o. o.

ul. Warszawska 23; 42-470 Siewierz, POLAND Phone:+48-(0)32-6705045 Fax:+48-(0)32-6713405 www.topcon-polska.pl

### TOPCON SINGAPORE MEDICAL PTE. LTD.

60 Alexandra Terrace, #08-27 The Comtech, SINGAPORE 118502 Phone:+65-68720606 Fax:+65-67736150 www.topcon.com.sg

### TOPCON INSTRUMENTS ( MALAYSIA ) SDN.BHD.

No. D1, (Ground Floor), Jalan Excella 2, Off Jalan Ampang Putra, Taman Ampang Hilir, 55100 Kuala Lumpur, MALAYSIA Phone:+60-(0)3-42709866 Fax:+60-(0)3-42709766

### TOPCON INSTRUMENTS ( THAILAND ) CO.,LTD.

77/162 Sinnsathorn Tower, 37th Floor, Krungthonburi Rd., Klongtongsai, Klongsarn, Bangkok 10600, THAILAND Phone:+66(0)2-440-1152~7 Fax:+66-(0)2-440-1158

### TOPCON CORPORATION BEIJING OFFICE

Block No.9, Kangding Street, Beijing Economic-Technological Development Area, Beijing,100176, CHINA Phone:+86-(0)10-6780-2799 Fax:+86-(0)10-6780-2790

### TOPCON CORPORATION SHANGHAI OFFICE

14L Huamin Empire Plaza, No.726, Yan-an Xi Road, Shanghai, 200050, CHINA Phone:+86-(0)21-5238-7722 Fax:+86-(0)21-5237-0761

### TOPCON CORPORATION BEIRUT OFFICE

P.O.Box 70-1002 Antelias,Beirut, LEBANON Phone:+961-4-523525/523526 Fax:+961-4-521119

### TOPCON CORPORATION DUBAI OFFICE

P.O.Box 293705, Dubai Airport Free Zone L.I.U J-12, Dubai, U.A.E. Phone:+971-4-299-5900 Fax:+971-4-299-5901

---

## TOPCON CORPORATION

75-1 Hasunuma-cho,Itabashi-ku,Tokyo,174-8580 Japan.

Phone:3-3558-2520 Fax:3-3960-4214 www.topcon.co.jp